

Dear reviewers,

This combined pdf file gathers the point-by-point response to the 3 reviews and the marked-up revised manuscript as display in the table of contents below.

Accordingly to our response to the first specific comment of reviewer 1, the title of the manuscript was changed to:

“A gain-loss framework based on ensemble flow forecasts to switch the urban drainage-wastewater system management towards energy optimization during dry periods.”

Table of Contents

Review 1 point-by-point response 2
Review 2 point-by-point response 8
Review 3 point-by-point response 11
Revised manuscript with track change..... 13

We would like to express our sincere thanks to the reviewers for their constructive comments and identification of areas in the manuscript which needed clarification.

On behalf of all the authors,

Vianney Courdent

Dear reviewer,

We greatly appreciate the review and acknowledge that the comments and suggestions will lead to an improved paper.

Please find in the table below our point-by-point response to the comments.

Referee # 1	
General comments	
<p><i>The manuscript presents an interesting topic within the scope of the journal. While enough information on the used methodology is given to enable a rough understanding, the reader will not be able to reproduce the applied methods based on that information. Result interpretation will be difficult for the reader without more specific information on the used hydrological model (its calibration and accuracy) [1] and the WWTP and the potential impact of the described method on its performance in terms of energy consumption and effluent water quality [2].</i></p>	<p>[1] Section 2.3 (P5&6) was split in 2, the first on the study case was expended with more data on the WWTP and the second on the hydrological model was further developed. The relation with the previous article (Courdent et al., 2016) which further described the model was made clearer.</p> <p>As suggested in the specific comment 19, the model output based on rain gauge data input will be added on figure 9 to illustrate the performance of the hydrological model.</p> <p>Courdent, V., Grum, M. and Mikkelsen, P. S.: Distinguishing high and low flow domains in urban drainage systems 2 days ahead using numerical weather prediction ensembles, J. Hydrol., doi:http://dx.doi.org/10.1016/j.jhydrol.2016.08.015, 2016.</p> <p>[2] Further information on the WWTP energy consumption was added in the study case section (P4 L34ff) and additional information was added to the results and discussions section (P9 L37ff).</p> <p>We do not have precise data regarding the impact on the effluent water quality. However the effluent water quality is of primary interest. The Danish WWTPs pay taxes on their effluent pollution load. Therefore the boundaries of the energy optimization scheme will be defined to respect the performance of the WWTP.</p> <p>Halvgaard et al. (submitted 2017), presents a control method that takes the effluent quality (nitrogen) into account. A reference to this article was added to the outlook section (P10 L23ff).</p> <p>R. Halvgaard, L. Vezaro, P. S. Mikkelsen, M. Grum, T. Munk-Nielsen, P. Tychsen, H. Madsen: Integrated Model Predictive Control of Wastewater Treatment Plants and Sewer Systems in a Smart Grid, Computer</p>

	<p>& Chemical Engineering, submitted 2017.</p>
<p><i>More information in the results section on the performance of the proposed method and a discussion of its risks and benefits would be very desirable as without them it is difficult to draw clear conclusions about the value of the method [3].</i></p>	<p>[3] The scope of this article is to develop a method to determine when the IUDWS management can be switched to optimizing its energy consumption, which is possible during dry weather (flow below a given threshold).</p> <p>As mentioned in the updated outlook section (P10 L23ff), Halvgaard et al. (submitted 2017) presents a Model Predictive Control (MPC) to control the power consumption of pumps in a sewer system and the treatment power consumption according to electricity prices and effluent quality (nitrogen). This article is currently under review for the Computer & Chemical Engineering journal.</p> <p>We agree that further information on results and performance would be appreciated and we are currently working towards it. As mentioned in the updated outlook section (P10 L 19), two large pipes will be constructed just before the inlet to the Damhusåen WWTP with the primary purpose to reduce CSO to cope with new regulations. These 2 pipes can contain a volume corresponding to one day of dry weather flow and would nicely fit the concept developed in this paper and in the paper by R. Halvgaard et al. (submitted 2017)</p>

<p>Specific comments</p>	
<p>1. P1 L1: This is one long title. Would “Coupling urban drainage-wastewater systems and electric smart grids during dry periods” not suffice? Even then I find the title somewhat misleading: Is the WWTP not continuously coupled to the smart grid? If I understand correctly, rather than coupling and uncoupling, only the temporal amount of energy consumption is optimized depending on the hydraulic condition.</p>	<p>The title was changed to :</p> <p>“A gain-loss framework based on ensemble flow forecasts to switch the urban drainage-wastewater system management towards energy optimization during dry periods.”</p>
<p>2. P2 L8ff: Maybe I misunderstand this sentence, but it seems to suggest that only because rain only occurs 7 % of the time it makes sense to look into energy optimization. Would it make less sense if you had 10 % of rain? Could you clarify/rephrase this?</p>	<p>P2 L8ff The sentence was modified for more clarity.</p>
<p>3. P2 L8ff: Dry weather flow rarely can be defined by</p>	

<p>“no rain”, usually (sufficient sewer network size and event intensity) wet weather conditions will be predominant for several hours after a rain event has ended (as the proposed method does by using the flow rather than the rain as a trigger for switching between control objectives). I suggest rephrasing this section accordingly.</p>	
<p>4. P2 L10ff (same phrase again, sorry): Striving for energy optimization and emission reduction of WWTP is standard practice for many years – both during dry and wet weather. With this background in mind it would be better to slightly rephrase and cite some relevant literature here to avoid this phrase being interpreted as a novel suggestion as such.</p>	
<p>5. P3 L15ff: Some details are discussed here that re-occur in section 3. Delete here?</p>	<p>As suggested this part was deleted to avoid reoccurrence.</p>
<p>6. P4 L5: A clear(er) definition of REV (as eg in the abstract) would be critical here as it forms the basis of the paper</p>	<p>P4 L2ff A sentence was added to describe the REV with more clarity.</p>
<p>7. P5 L20ff: Are methods (i) and (ii) defined in literature? They seem to be a mix of other methods. It would not be possible to reproduce your method from this section. Please give more specific information on the used methods for enhancing the forecast.</p>	<p>P5 L17: The reference to the just published manuscript (Courdent et al. 2016) was made clearer.</p>
<p>8. P6 section 2 and especially 2.2 discusses methods. I'd suggest to move these parts to section 3</p>	<p>The NWP post-processing methods described in section 2.2 are developed in the previous manuscript (Courdent et al. 2016) and are used to generate input data to the model for this article.</p> <p>It was decided to develop it under the data section to distinguish it from the core methods of this paper.</p>
<p>9. P6 L20ff: You mention that the DWF module of the model is calibrated, but there are no details on the calibration of the Nash cascades. These details seem essential for accurate predictions, please add them to this section.</p>	<p>P6 L20ff As mentioned in the general comments [1] this section was be split in 2 to further describe the hydrological model, and the link to the previous article (Courdent et al. 2016) developing the hydrological model was made clearer.</p>
<p>10. P5, section 2.3: No details on the WWTP and its energy consumption are given while this forms the focus of the paper [1]. Changed flow regimes at the influent will necessarily cause changes in energy consumption of the WWTP. How are these considered</p>	<p>[1]As mentioned in the reply to general comments, section 2.3 was be split in 2 and further details on the WWTP were added in the study case section (P6 L1).</p> <p>[2] Indeed, the control of the energy consumption</p>

<p>in this study? [2]</p>	<p>based on the energy market can result in a decrease of the cost together with an increase of the energy consumption as explained in the added reference (Aymerich et al., 2015) in P12 L23ff.</p> <p>This aspect is out of the scope of this article. We added in the outlook section (P13 L11ff) a reference to (Halvgaard et al., submitted 2017) which is currently under review. This article presents a Model Predictive Control (MPC) to control the power consumption of pumps in a sewer system and the treatment power consumption according to electricity prices</p> <p>Aymerich, I., Rieger, L., Sobhani, R., Rosso, D., Corominas, L., 2015. The difference between energy consumption and energy cost: Modelling energy tariff structures for water resource recovery facilities. <i>Water Res.</i> 81, 113–123. doi:10.1016/j.watres.2015.04.033</p>
<p>11. P6 L31ff: Move to introduction?</p>	<p>This part of the section 2.4 on energy market section was moved to the introduction (P2 L17ff).</p>
<p>12. P7 L5ff: Leave out? Does not add anything to the understanding of the reader.</p>	<p>The introduction to the methodology section was removed.</p>
<p>13. P11 L5ff: are these not results that should be moved to the next section?</p>	<p>This part was moved to the result section (P11 L3ff).</p>
<p>14. Figure 8 is not interpreted in the text. Omit?</p>	<p>Figure 8 is mentioned in P12 L9.</p>
<p>15. P12 L13: How big are the uncertainties in the energy price forecasts? Could you comment on their (potential) influence on your method?</p>	<p>The term “forecasted” was changed for more clarity (P12 L10).</p> <p>The energy price for the incoming day is set through the energy market (Nord pool for Denmark) based on bids and offers and is therefore fixed without uncertainty.</p> <p>“Buyers and suppliers submit bids and offers for each hour of the next day and each hourly MCP (market clearing price) is set such that it balances supply and demand.” (Weron 2006)</p> <p>The smart grid section was reshaped, part of it was moved to the introduction (see reply to comment 11) and additional information on the electricity market were added (there are different electricity markets with different lead times, e.g. the day-ahead market have 24</p>

	<p>hours lead time whereas the intraday market has 1 hour lead time. Bids and offers made on the first market can be adapted on the second).</p> <p>Weron, R.: Modeling and forecasting electricity loads and prices: A statistical approach, First Edit., John Wiley & Sons Ltd., 2006.</p>
<p>16. P12 L15ff: In this scenario, it is possible to save 26 €MWh during 2 days. I suggest to add information that answers at least a number of the following questions in order for the reader to be able to understand the meaning of this result: Is this a representative result? What is the average/peak energy consumption of the WWTP? What is the maximum amount of energy that could be switched? How much could be saved during the 2 years of data you used? How does that impact the total energy consumption of the WWTP ('switching' could result in an increase as well as a decrease)? What is the influence on the WWTP effluent performance and emission of greenhouse gasses?</p>	<p>This comment is similar to general comments [2].</p> <p>Further information on the WWTP energy consumption (e.g. energy consumption per m³) was added to allow the reader to have a better understanding of the meaning of this result (P6 L1ff and P12 L15ff).</p> <p>As mentioned in the reply to comment 10 and 18, energy optimization based on the energy price can result in an increase of the total energy consumption. A references was added to underline this possibility (P12 L23).</p> <p>The energy consumption optimisation scheme (not developed in this article) has to include the WWTP performance within its decision criteria. E.g. (R. Halvgaard et al., submitted 2017) mentioned in the outlook (P13 L11ff) used the nitrogen concentration as a measure of effluent quality.</p> <p>The impact on emission of greenhouse gasses was not directly assessed. However, daily peaks in waste water usually coincide with peak demand on the power grid, thus coinciding with the highest energy price periods. Hence, reducing these wastewater inflow peaks when energy cost are high will also benefit the energy system by reducing grid load and GHG emissions (due to the need for more carbon- intensive energy sources during peak power demand periods).</p>
<p>17. P12 L15ff: What is the cost of the suggested system (at the least the NWP data will have to be purchased + some man-hours for keeping the real-time system up and running) as compared to its benefits? It seems these considerations should be included in order to judge the actual gains produced by the system.</p>	<p>A large project is currently under implementation on the downstream part of the study case catchment just before the inlet to the WWTP. Two large pipes with a storage volume corresponding to the daily dry weather flow to the WWTP will be constructed to cope with new regulations on CSO. The volume of these two pipes would nicely fir the concept developed in this article (P13 L7) and provide further information on the cost of the system.</p> <p>A reference to this project was added to the outlook</p>

	section (P10 L19ff)
<p>18. P12 L24 “optimization based on economic objectives will also yield environmental benefits”: This seems a much too broad statement that should be explained or based on a citation. In the context of this paper, it seems that it would be perfectly possible to create a scenario where ‘switching’ energy consumption would lead to an overall increase of energy consumption (e.g. by running the blowers on a frequency at which they are less efficient than when not ‘switching’), but a decrease in cost.</p>	<p>The intended message of this sentence is that the correlation between energy price and proportion of wind energy leads to the consumption of energy with a lower CO2 footprint. But indeed as you rightfully pointed out the optimisation can result in an increase of the overall energy consumption.</p> <p>The sentence was motivated to clarify this point (P12 L22ff).</p>
<p>19. P12 L26: “most EMs predict the high flow event but often too early” Is this a problem of the precipitation prediction or the hydrological model? This would be difficult for the reader to judge (without information on the calibration of the hydrological model). Maybe you could add a line in figure 9: the output of the hydrological model given the observed rain. This would also (more or less) address the above comment for P6 L20ff.</p>	<p>Figure 9 was updated accordingly.</p>
<p>Technical corrections</p>	<p>Thank you for the technical corrections, which are accommodated in this revised version of the manuscript.</p>

Dear reviewer,

We greatly appreciate the review and acknowledge that the comments and suggestions will lead to an improved paper.

Please find in the table below our point-by-point response to the comments.

Referee # 2	
General comments	
<p><i>The problem is exposed as a dynamic one (e.g. P4 L25-26, P9 L27-30, P14 L21-22). However it is solved as a static one: the relative economic value is presented as a function of the gain/loss ratio [1]. The decision threshold (i.e. the fraction of members of the ensemble of predicted discharge exceeding a discharge threshold) beyond which the manager decides to switch from energy optimization to safety of the system is deduced from the envelope of separate curves. As for the choice of a method for the post-processing of numerical weather prediction model the maximum threat method extends significantly the range towards low gain/loss ratios resulting in positive relative economic values compared with the aerial overlap method. Having these results, the methodology has still to be proven in real dynamic situation i.e. where the decision to be taken at a given time depends on the decisions already taken. What is missing in order to that? An order of magnitude of the losses in case of combined sewer overflow, a hydraulic model able to reflect the management actions? The authors are asked to make clear the scope of the paper and either add new results or add comments in the outlooks [2].</i></p>	<p>[1] Thank you to point this out, you are right. The use of the term “dynamic” was corrected for more clarity.</p> <p>The referenced articles on the REV (Richardson, 2000; Roulin, 2006) are using fixed alpha values (the cost of mitigation measures and their benefits are assumed fixed). In our case the alpha value varies with time, the gain depends directly on the variation of the energy market. Hence the incentive to optimize the IUDWS for energy consumption changes with time. In this sense the alpha ratio is dynamic. But, indeed for at a given time, for given NWP forecast the alpha is fixed and the problem solved as a static one.</p> <p>[2] We agree that further information on results and performance would be appreciated and we are working towards it. As mentioned in the updated outlook section (P10 L 19), two large pipes will be constructed just before the inlet to the Damhusåen WWTP with the primary purpose to reduce CSO to cope with the new CSO regulations. Those 2 pipes can contain a volume corresponding to one day of dry weather flow and would nicely fit the concept developed in this paper and in the paper by R. Halvgaard et al.</p> <p>R. Halvgaard, L. Vezaro, P. S. Mikkelsen, M. Grum, T. Munk-Nielsen, P. Tychsen, H. Madsen: Integrated Model Predictive Control of Wastewater Treatment Plants and Sewer Systems in a Smart Grid, Computer & Chemical Engineering, submitted 2017.</p>
<p><i>I missed information regarding the methodology. No lead time is specified with the results. Are all the ensembles (2 years x 4 issue hours) used at hourly time step to the forecast horizon of 54 hours (P5 L14-18)? Or 2 days (P3 L5, P12 L11-26)? How the scores are computed regarding both the issue time and the lead</i></p>	<p>[3] Indeed a decrease in the performance skill is observed with increasing lead time as was documented in (Courdent, 2016). The bids and offers on the daily energy market are made up to 36 hours in advance. Therefore, the different lead times are aggregated in the results. This point was added in the methodology</p>

<p><i>time? In case the forecast horizon is 2 days, how do the authors deal with the decreasing skill scores or relative economic value of the predictions with the lead time? [3]</i></p>	<p>section (P6 L2ff).</p>
--	---------------------------

<p>Specific comments</p>	
<p>1. P3 L26 “spatial” instead of “special”. Do you have a reference for this assertion?</p>	<p>Indeed it is a typo, we meant “spatial”. This misspelling was corrected.</p>
<p>2. P4 L1 “The radius of the neighbouring area included is used as a parameter during the decision making, in addition to fEM.” should move from introduction to the methodology section (2 Material: : : 2.2). P11 L18, Figure 7 Results considering a radius of 6 grid cells are presented. This radius has been optimized on REV? What is the sensitivity to this parameter?</p>	<p>The radius was not specifically optimised on REV, the selected radius was based on the previous article (Courdent et al., 2016), which describes this method further.</p>
<p>3. P5 L14 UTC</p>	<p>UTC was added to the NWP generation time.</p>
<p>4. P6 L18 and other occurrences of “forecasted” should be “forecast”. “summing up to a total of n event assessments” : this part of the description methodology should be made much clearer (see general comments).</p>	<p>The occurrences of “forecasted” were corrected to “forecast”.</p> <p>As mention in the reply to the general comment [3], the description of an event was made clearer in the methodology section (P6 L2ff).</p>
<p>5. P7 L4 “Methodology” : section 2 involves also description of the methodology. Section 3 is more related with validation.</p>	<p>This comment is similar to the reviewer 1 specific comment [8].</p> <p>The NWP post-processing methods described in section 2.2 are developed in the previous manuscript (Courdent et al. 2016) and are used to generate input data to the model for this article.</p> <p>Despite being a method, it was decided to develop it under the data section to distinguish it from the core methods of this paper. This section was modified to make this clearer.</p>
<p>6. P10 L6 and other occurrences (e.g. Table 5, Figure 5, 8) “always optimize”, “never optimize” sounds strange because the paper is all about optimization. Find a short reference to the two objectives (like “always energy objective”). 1/21/2</p>	<p>We agree the text on the figure a will be changed for more clarity.</p>

<p>7. P11 L20-29, Figure 7b, Table 4 The slightly better upper bound provided by the areal overlap method can't be seen on the figure. How the complementarity of both post-processing approaches can be used in a real situation? Through the gain/loss ratio and the decision threshold?</p>	<p>The complementarity of the 2 approaches is more visible on the ROC diagram Figure 7a. The catchment areal overlap provides valuable information for low PoFD, which are not covered by Maximal threat approach.</p> <p>This is not especially visible on the REV diagram Figure 7b due to the logarithmic scale and the allocated value to the different outcomes (Table 3) (i.e. no actions are taken in case of positive forecast and therefore no value is allocated to hits and false).</p> <p>With another definition of decision making, the complementary could be more pronounced. E.g. REV on mitigation measures (e.g. flood prediction) will allocate the values differently and false alarms may have a high impact.</p>
<p>8. P12 L15-18 “can yield up to 8 €” what is the order of energy consumption we are dealing with? What is missing is an overall estimation of the cost of energy during the 2 years and how much is gained during the same period using the switching strategy optimized based on REV results.</p>	<p>This comment is similar to the specific comment [16] of Reviewer 1.</p> <p>Further information on the WWTP energy consumption (e.g. energy consumption per m³) was added in the case study section (P4 L34ff) and in the results section (P9 L37ff).</p> <p>The aim of this article is to provide a framework using EPS NWP to predict when a management switch to IUWDS is beneficial considering the uncertainty of the weather forecast. As mentioned in the updated outlook section (P10 L23ff), the control strategy needed for the optimisation scheme is developed in another manuscript by R. Halvgaard et al. currently under review.</p> <p>R. Halvgaard, L. Vezzaro, P. S. Mikkelsen, M. Grum, T. Munk-Nielsen, P. Tychsen, H. Madsen: Integrated Model Predictive Control of Wastewater Treatment Plants and Sewer Systems in a Smart Grid, Computer & Chemical Engineering, submitted 2017.</p>
<p>9. P24 Figure 9(a) Add a legend for the two curves.</p>	<p>The meanings of the two curves are described by the axis label and colour, a legend was added for more clarity.</p>

Dear reviewer,

We greatly appreciate the review and acknowledge that the comments and suggestions will lead to an improved paper.

Please find in the table below our point-by-point response to the comments.

Referee # 3	
General comments	
<p><i>I can find little to fault the paper. My main query would be that I could find no details or reference as to how the system is operated during the 'optimised' phase apart from relatively vague statements. While the paper is interesting without this, it does limit the understanding / reproducibility. I can see that the omission of this may be due to commercial reasons given the authors' affiliations, but it would be useful to explicitly state this.[1]</i></p>	<p>[1] The aim of this article is to provide a framework using EPS NWP to predict when a management switch to IUWDS is beneficial considering the uncertainty of the weather forecast. As mentioned in the updated outlook section (P10 L23ff), the control strategy of an optimisation scheme is developed in another manuscript by R. Halvgaard et al. currently under review for the Computer & Chemical Engineering journal.</p> <p>R. Halvgaard, L. Vezaro, P. S. Mikkelsen, M. Grum, T. Munk-Nielsen, P. Tyhsen, H. Madsen: Integrated Model Predictive Control of Wastewater Treatment Plants and Sewer Systems in a Smart Grid, Computer & Chemical Engineering , submitted 2017.</p>
<p><i>It would also be useful to understand more details of the calibration of the hydrological model even if just a few short sentences. [2]</i></p>	<p>[2] This comment is similar to the general comment [1] and the specific comment [10] from the first reviewer.</p> <p>[1] Section 2.3 (P5&6) was split in 2, the first on the study case was expended with more data on the WWTP and the second on the hydrological model was further developed. The relation with the previous article (Courdent et al., 2016) which further described the model was made clearer.</p> <p>Courdent, V., Grum, M. and Mikkelsen, P. S.: Distinguishing high and low flow domains in urban drainage systems 2 days ahead using numerical weather prediction ensembles, J. Hydrol., doi:http://dx.doi.org/10.1016/j.jhydrol.2016.08.015, 2016.</p>
<p><i>While clearly outside the scope of this paper, it would be of great interest to see any results from a real world implementation of the proposed framework should it be implemented! [3]</i></p>	<p>[3] We agree that further information on results and performance would be appreciated and we are working towards it. As mentioned in the updated outlook section (P10 L 19), two large pipes will be constructed just before the inlet to the Damhusåen WWTP with the</p>

	<p>primary purpose to reduce CSO to cope with the new CSO regulations. Those 2 pipes can contain a volume corresponding to one day of dry weather flow and would nicely fit the concept developed in this paper and in the paper by (R. Halvgaard et al., submitted 2017)</p>
--	---

A gain-loss framework based on ensemble flow forecasts to switch the urban drainage-wastewater system management towards energy optimization during dry periods.

Vianney Courdent^{1,2}, Morten Grum^{1,†}, Thomas Munk-Nielsen¹, Peter S. Mikkelsen²

¹ Krüger Veolia, Søborg, 2860, Denmark

² Department of Environmental Engineering, Technical University of Denmark, Kgs. Lyngby, 2800, Denmark

[†] Present address: Founder and CEO of WaterZerv, Environmental Services, Denmark.

Correspondence to: Vianney Courdent (vatc@env.dtu.dk)

Abstract. Precipitation is the major perturbation to the flow in urban drainage and wastewater systems. Flow forecasts, generated by coupling rainfall predictions with a hydrologic runoff model, can potentially be used to optimise the operation of Integrated Urban Drainage-Wastewater Systems (IUDWS) during both wet and dry weather periods. Numerical Weather Prediction (NWP) models have significantly improved in recent years; increasing their spatial and temporal resolution. Finer resolution NWP are suitable for urban catchment scale applications, providing longer lead time than radar extrapolation. However, forecasts are inevitably uncertain and fine resolution is especially challenging for NWP. This uncertainty is commonly addressed in meteorology with Ensemble Prediction Systems (EPS). Handling uncertainty is challenging for decision makers and hence tools are necessary to provide insight on ensemble forecast usage and to support the rationality of decisions (i.e. forecasts are uncertain therefore errors will be made, decision makers need tools to justify their choices, demonstrating that these choices are beneficial in the long run).

This study presents an economic framework to support the decision making process by providing information on when acting on the forecast is beneficial and how to handle the EPS. The Relative Economic Value (*REV*) approach associates economic values to the potential outcomes and determines the preferential use of the EPS forecast. The envelope curve of the *REV* diagram combines the results from each probability forecast to provide the highest relative economic value for a given gain-loss ratio. This approach is traditionally used at larger scales to assess mitigation measures for adverse events (i.e. the actions are taken when events are forecast). The specificity of this study is to optimise the energy consumption in IUDWS during low flow periods by exploiting the electrical smart grid market (i.e. the actions are taken when no events are forecast). Furthermore, the results demonstrate the benefit of NWP neighbourhood post-processing methods to enhance the forecast skill and increase the range of beneficial use.

1 Introduction

The primary objective of combined urban drainage systems (UDS) and wastewater treatment plants (WWTP) is to convey and treat waste water and to prevent flooding and combined sewer overflows (CSO). In order to achieve these objectives pipes and detention basins in combined UDS are dimensioned to cope with relatively large rain events. Typically, surcharge of manholes and flooding is only allowed to occur on average every 10 years (as on the Danish regulations, (Harremoës et al., 2005)) whereas overflow occurs more frequently depending on the local environmental regulations, from e.g. 10 times per year to once in 10 years. This means that during dry weather the flow is relatively low compared with the conveyance capacity of the UDS and that the storage capacity is left unused. Rainfall only occurs rarely, e.g. on the study case catchment (more details in Sect. 2.3.) the raining period represents 7.2% of the time. Hence Integrated Urban Drainage-Wastewater Systems (IUDWS) are mostly under low flow conditions. During these periods the IUDWS management objective can be

Deleted: Coupling urban drainage-wastewater systems and electric smart grids during dry periods: A gain/loss framework using the relative economic value with ensemble flow forecasts to predict the switch between management objectives¶

Deleted: ed

Deleted: ed

Deleted: Rainfall only occurs rarely, on average 7.2 % of the time in the Damhuså catchment, Copenhagen (more details in Sect. 2.3.), which means that during dry weather, the management objectives of Integrated Urban Drainage-Wastewater Systems (IUDWS) could potentially be switched from the normal operational focus on CSO and flood prevention to other goals like minimization of energy consumption and reduction of CO₂ emissions.

switched from its priority operational focus on CSO and flood prevention towards other goals like energy consumption and CO2 emissions.

Denmark has the political ambitions to have a fossil fuel free energy system by 2050 which requires the development of renewable energy sources (Ministry of Foreign Affairs of Denmark, 2016). A main critic towards renewables like wind and solar energy is their intermittent nature. Therefore a key parameter for the transition to a green energy system is the implementation of an electric Smart Grid with flexible, proactive consumers to balance the fluctuating power production (Hadjsaid and Sabonodiére, 2012). The European Technology Platform for Smart Grids defines the concept of Smart Grids as an “electricity network that can intelligently integrate the actions of all users connected to it - generators, consumers and those that do both - in order to efficiently deliver sustainable, economic and secure electricity supplies” (www.smartgrids.eu/). Energy markets are developed, as part of the Smart Grid, to align electricity production and consumption through bids and offers. Hence the electricity price is based on supply and demand, creating an economic incentive to distribute the energy consumption in time (e.g. shifting non-essential energy consumption out of the consumption peaks). For further detailed history and description of electricity markets see (Weron, 2006).

IUDWS can potentially be used actively to take advantage of the energy market variation. Wastewater for example contains organic matter which can be converted to biogas at the WWTP, and the biogas production process may provide some energy storage that is potentially useful in a smart grid context. Furthermore, during dry periods, the unused storage in the UDS can be used as buffer to control the timing of the energy consumption associated with wastewater transportation and treatment. Figure 1 highlights that both wastewater production and energy consumption are driven by human activities and therefore have similar daily pattern. This means that the energy is generally more expensive when the need for wastewater transportation and treatment is peaking. The energy market is also influenced by other parameters (e.g. the solar and wind intensity) but on yearly average the impact of the daily consumption can be observed.

Aymerich et al. (2015) investigated the relation between the energy consumption and energy cost at a WWTP in regard to energy tariff structures (i.e. energy markets). The aeration process represents between 50 and 70 % of the WWTP process energy consumption (Rosso and Stenstrom, 2005). Leu et al. (2009) studied the impact of a varying wastewater load on the oxygen transfer efficiency and aeration costs considering to the daily variation of the power rates and showed a potential to reduce the average power costs, within the limitations of the WWTP storage capacity. Bjerg et al. (2015) investigated the use of the storage volume in the pipe system upstream from a WWTP in Kolding (Denmark) to store wastewater and utilise the energy price fluctuations. However, such optimization requires information on the incoming loads (i.e. flow predictions) to know when it is safe to optimise the energy consumption (i.e. when it is dry weather) and when to prepare and operate the IUDWS to cope with large inflows during wet weather. Such flow predictions should ideally cover the forecast horizon of the smart grid market, i.e. 1 to 2 days (e.g. day-head energy market (Zugno, 2013)), which requires the use of Numerical Weather Prediction (NWP) models.

NWPs are already in use in other fields such as wind and solar power production prediction (Bacher et al., 2009; Giebel et al., 2005), streamflow forecasting (Cuo et al., 2011; Shrestha et al., 2013), reservoir inflow prediction (Collischonn et al., 2007), flood forecasting (Damrath et al., 2000) and typhoon forecasting (Chang et al., 2015). Uncertainty is a challenge for NWPs especially for precipitation which is non-continuous and highly variable in both space and time. To tackle this problem meteorologists commonly generate Ensemble Prediction Systems (EPS) by perturbing the initial conditions and the physics of the NWP models to generate a number of ensemble members (EM) that represent an ensemble spread. The quality of an EPS can be quantitatively assessed based on various forecast characteristics. The relative operating characteristic (ROC) (Mason, 1982) is used to measure the discrimination skill (i.e. the ability to discriminate events and non-events) of an EPS, by plotting the empirical Probability of Detection (PoD) versus the Probability of False Detection ($PoFD$). Using an EPS increases the event discrimination skill by providing a larger range of predictions than an individual deterministic forecast.

Deleted: t

Deleted: detain

Deleted: z

Deleted: Each fraction of ensemble members f_{EM} from $1/N$ to 1 (with N the number of EMs) provides a set of prediction skills. Choosing a value of f_{EM} converts the EPS to a single forecast which treats forecast with a probability greater than f_{EM} as the occurring event. For example, for $f_{EM} = \frac{1}{N}$ then at least 1 EM must predict an event for the general prediction to be an event, and for $f_{EM} = 1$ then all the EMs must predict an event for the general prediction to be an event (Courdent et al., 2016).

The development of high-resolution limited area NWP models has led to more realistic-appearing forecasts. Convective precipitations are described in an explicit and more detailed way using mesoscale atmospheric processes (Sun et al., 2014). These developments foster the opportunity of UDS applications which require fine temporal and spatial resolution. However precipitation is one of the most difficult variables to forecast on an urban scale due to its large variability in space, time and intensity (Du, 2007). Precipitation forecast uncertainties increase rapidly with decreasing spatial grid size as inevitable errors in position and timing of rain cells are amplified with the increase in resolution. EPS aim at describing this uncertainty, but EPS are generally underdispersive and unable to capture all sources of uncertainty. NWP post-processing methods (also called pre-processing from a hydrological modelling point of view) are thus necessary to obtain reliable probabilistic forecast as explained in (WWRP/WGNE 2009). Courdent et al. (2016) described NWP post-processing methods for urban drainage flow forecasting and compared their event discrimination skills. The neighbourhood methods (Theis et al., 2005) can e.g. be used to enhance the forecast skill by accounting for potentially misplaced rain events. The maximal threat method NWP post-processing, used in this study, considered the highest rainfall prediction within a given area surrounding the catchment. The radius of the neighbouring area included is used as a parameter during the decision making, in addition to f_{EM} . This article presents a framework for objectively optimizing EPS forecast-based decision making in management of IUDWS by selecting the decision threshold f_{EM} and post-processing neighbourhood method given the specific problem at hand. The Relative Economic Value (REV) approach associates economic values to the outcomes of the decision system and assesses the forecast value relatively to potential benefit resulting from a perfect forecast. The preferential management for a given EPS forecast is characterised by the highest REV. As example we considered the decision problem of switching from normal operation focusing on flow management to dry weather operation focusing on energy optimization linking with the Smart Grid. To measure the usefulness of weather forecasts, the forecast skills have to be converted to potential economic benefits for the user decision making process. Richardson (2000) used the *REV* to assess the economic benefit of road gritting to prevent the formation of ice using weather models in comparison to using purely climatological information (i.e. the statistical behaviour of the weather, e.g. the return period of an event). Economical values were assigned to the different prediction outcomes described in a contingency table: (a) hits, (b) false alarms, (c) misses and (d) correct negatives. These economic values represent the benefit of taking actions (or non-action) when the forecast reveals to be correct against the drawbacks of those actions (or non-action) in case of forecast error. EPS provides a range of prediction skills characterised by the combined choice of post-processing method and decision threshold (f_{EM}) used to predict an event. The *REV* of each combination is quantified considering the occasions when the forecast proves to be beneficial, detrimental or neutral to the user and the economic value associated with these situations. The higher the cost of inappropriate action relative to the potential gain, the more certainty the user requires about the forecast before he/she takes action. Previous studies on *REV* analysis typically assessed the benefit of prevention measures mitigating severe weather events, such as frost (Richardson, 2000), intense precipitation (Atger, 2001), river floods (Roulin, 2006) and typhoons (Chang et al., 2015), expressed as a cost-loss ratio. This study develops a different perspective, assessing the potential benefit of optimizing IUDWS when the forecast predicts periods with low flow (i.e. dry weather when no events are forecast). Therefore our decision model is not based on a cost-loss ratio but a gain-loss ratio. Furthermore the mentioned studies consider a fixed ratio whereas in our case, (i) the gain depends on smart grid variations and (ii) the loss is related to the risk of Combined Sewer Overflow (CSO) and the negative impact on the WWTP operation. Hence the gain-loss ratio and the optimum combination of post-processing method and decision threshold need to be reassessed for each time step. This paper is organized as follows: section 2 introduces the DMI-HIRLAM-S05 weather model used to produce the data used in our study, the used post-processing method and the hydrological rainfall-runoff model used. Section 3 describes the prediction performance evaluation methods used, including the ROC and the *REV* diagrams. Results and prediction examples are presented and discussed in section 4 and finally, section 5 provides the conclusions.

Deleted: have

Deleted: special

Deleted:

Deleted: with the highest Relative Economic Value (REV)

Deleted: ;

Deleted: a

Deleted: ed

2 Material: NWP data, study case and hydrological model

As emphasized by Shrestha et al. (2013) the evaluation of NWP model precipitation forecasts for streamflow forecasting should be done with a hydrological perspective. Therefore as recommended by Pappenberger et al. (2008), the evaluation of urban drainage flow forecasts is in this paper based on a coupled meteorological and hydrological model. Hence, the forecast skills are assessed based on discharge predictions and discharge observations rather than precipitation forecasts and precipitation observations. This methodology considers the importance of the dominant hydrological processes and the non-linear error transformation by the hydrological model.

This section describes the Numerical Weather Prediction (NWP) model and data used in the study. Then the post-processing neighbourhood methods are presented, the urban catchment study case is presented and the hydrological model is described and finally, the energy market data used is presented.

Deleted: used of

Deleted: is

Deleted: d

2.1 The EPS HIRLAM-DMI-S05 Numerical Weather Prediction (NWP) model

The rainfall forecasts used in this study were generated by the DMI-HIRLAM-S05 model and were provided by the Danish Meteorological Institute (DMI). This NWP model has a horizontal resolution of 0.05° (approx. 5.6 km) and a forecast horizon of 54 hours with hourly time step predictions. New forecast are generated every 6 hours at 0h, 6h, 12h and 18h UTC. The DMI-HIRLAM-S05 ensemble is a 2-dimensional EPS comprising 25 members based on 5 different initial conditions and 5 different model structures. For further description of the processes and parameters mentioned above, see the HIRLAM technical documentation (Uden et al., 2002), the DMI technical report (Feddersen, 2009) and the HIRLAM website (<http://www.hirlam.org/>). The study uses 2 years of archived EPS NWP data (from June 2014 to May 2016).

2.2 Enhancing forecast by post-processing NWP EPS data

Two NWP post-processing methods developed in (Courdent et al., 2016) were used in this study: (i) the realistic catchment “weighted areal overlap” method which only considers the grid cells overlapping the hydrologic catchment and weighs them based on the percentage of overlap and (ii) the “maximal threat” in the surroundings method which considers cells within a defined radius around the catchment. The maximal threat method combines the worst scenario approach and the neighbourhood method developed by Theis et al. (2005), and accounts for neighbourhood cells in the prediction as illustrated by Figure 2. Hence, the maximal threat approach considers as input, for each ensemble member, the highest rainfall intensity in the surroundings. This method keeps the same ensemble size as the weighted areal overlap method and reduces the number of missed events but increases the number of wrongly or over-predicted events.

Deleted: ,

Deleted: (Courdent et al., 2016)

Deleted: and hydrological model description

2.3 Study case

The economic framework developed in this study was applied on the Damhuså urban drainage catchment (Copenhagen, Denmark). This highly urbanised area with compact residential housing is equipped with a combined sewer system which conveys wastewater, rainfall runoff from paved surfaces and infiltration inflow especially in the winter months. This catchment was chosen for the absence of major flow control infrastructures affecting its hydraulic response in order to simplify the modelling approach needed for our demonstration. The Damhusåen WWTP has a capacity of 350 000 PE. Its biological treatment has a maximal hydraulic capacity of 10,000 m³/h. In 2015, the WWTP treated 33.39 mio. m³ and consumed 8,735 MWh of electricity which correspond to a ratio of 0.261 kWh/m³. In parallel the WWTP produced 8,735 MWh of heat and 211 MWh of electricity from its biogas engine (BIOFOS, 2015).

Rainfall observation data were obtained from the national Danish SVK rain gauge network (blue circles on Figure 3 which is operated by the Danish Meteorological Institute (DMI) and the Water Pollution Committee of the Danish Society of Engineers (SVK – Spildevandskomiteen, in Danish). The rainfall measurements were recorded with a 1 minute temporal and a 0.2 mm volumetric resolution, for more information see (Jørgensen et al., 1998). The catchment outlet (red hexagon on

Figure 3) is a combined sewer pipe interceptor with a maximum capacity of $10,000 \text{ m}^3 \text{ h}^{-1}$. Once this threshold is reached CSOs occur. The overflowing water is discharged untreated into a nearby small river (Damhusåen) while the remaining flow is discharged through the interceptor pipe which is monitored using an electromagnetic flow meter with a 2 minutes temporal resolution and operated by the utility company HOFOR.

5 This study is based on event prediction by characterising the flow status in the IUDWS and distinguishing two domains, (i) periods with high flows during which the management objective is to maximize the hydraulic capacity of the WWTP to limit the impact of CSO etc. and (ii) periods with low flows during which the management objectives can be switched to WWTP operational efficiency, minimizing energy consumption, etc. The event definition should be evaluated relatively to the specific IUDWS and low-flow optimisation scheme in focus. In this study the occurrence of an event is defined by a flow
10 exceedance of $4,000 \text{ m}^3 \text{ h}^{-1}$ over a 1 hour period. For each NWP, the occurrence (or non-occurrence) of a high flow event is assessed for each hourly time step forecast.

2.3 Hydrological model description

The hydrological model is composed of 3 main conceptual parts: (i) the wastewater flow from households is modelled using 2nd-order Fourier series, see e.g. (Langergraber et al., 2008), (ii) the fast rainfall-runoff from impervious areas is represented
15 by a lumped conceptual model using the Nash linear reservoir cascade concept (Nash, 1957) and (iii) the slow runoff (caused e.g. by infiltration-inflow) is also modelled based on the Nash linear reservoir cascade concept using a wetness index characterised by the monthly potential evaporation and previous rainfall events. This hydrological model is further detailed in (Courdent et al., 2016). The wastewater flow parameters were estimated first, using flow observations from summer
20 periods without rainfall events to avoid influence from the two other processes. Then, using fixed wastewater parameters, the parameters of the fast rainfall-runoff were estimated based on rain and flow data for rain events during summer months to avoid influence from the slow runoff process, which was calibrated last for the full period (from November 2012 to November 2014). In all cases the calibration was conducted using the Differential Evolution Adaptive Metropolis (DREAM) method (Laloy and Vrugt, 2012) considering the root mean square error as objective function.

2.4. Energy market data

25 This study used historical data from the day-ahead energy market provider Nord Pool. The day-ahead market has 24 hours lead time. Buyers and suppliers submit bids and offers for each hour of the next day and each hourly market clearing price is set such that it balances supply and demand. The intraday market which only has 1 hour lead time is acting as a balancing market to support the day-ahead market. The hourly energy prices are defined over a geographical area. The geographical area corresponding to our case study is DK2 which covers the entire Zealand (<http://www.nordpoolspot.com/>).

3 Methodology

3.1 Contingency table

The probability that the flow will exceed a given threshold is estimated as the fraction of EMs predicting an event. The ensemble (probability) forecast can be converted to a single binary forecast by selecting a decision threshold (f_{EM}) (threshold probability). If the fraction of ensemble members (EM) predicting an event is higher or equal to the decision
35 threshold (f_{EM}) then an event is forecast.

The empirical performance over a period of time of a binary forecast can be summarized in a 2x2 contingency table showing the number of correctly and incorrectly forecast events occurring or not occurring (Table 1). Hits (a) represent the correct positives, false alarms (b) represent the false positives, misses (c) represent the false negatives and the correct negatives (d) represent the correct forecasts of no events occurring. Measures of performance of a sequence of binary forecasts can be

- Deleted: T
- Deleted: ed
- Deleted: (summing up to a total of n event assessments).
- Deleted: calibrated to dry weather flow observations (Fig. 1)
- Deleted: , see
- Deleted: details
- Deleted: ¶
- Deleted: Power systems are experiencing considerable changes, facing a paradigm shift from a centralized network delivering one-directional electricity to a distributed network with active consumers. Indeed, new energy sources, e.g. wind, solar, biomass and cogeneration plants (combined heat power), are spatially highly distributed. Furthermore, renewable energy sources (wind and solar power) are characterized by high temporal variability and uncertainty over production levels which have significant impact on other sources to protect the integrity of the network (Hadjsaid and Sabonnodièrè, 2012). The electric smart grid aims at facing these challenges. The European Technology Platform for Smart Grids defines the concept of Smart Grids as an “electricity network that can intelligently integrate the actions of all users connected to it - generators, consumers and those that do both - in order to efficiently deliver sustainable, economic and secure electricity supplies” (www.smartgrids.eu/).
- Deleted: market
- Deleted: E
- Deleted: per hours
- Deleted: ,
- Deleted: t
- Deleted: ¶
- Deleted: The methods used in this study are mainly borrowed from the field of meteorology and further developed to match the needs in IUDWS management. This section is divided in three parts. First the contingency table, PoD and $PoFD$ are introduced and the Brier Skill Score (BSS) is presented. Then the ROC diagram which displays the discrimination skill of an EPS is explained. Finally the Relative Economic Value method which translates PoD and $PoFD$ of an EPS into an economic value of the forecast is explained and adapted from a cost/loss to a gain/loss ratio basis. ¶
- Deleted: ed
- Deleted: ed

formulated as a function of these four outcomes (a , b , c and d). Those 4 possible outcomes sum up to n which corresponds to the total number of events assessed. Each event corresponds to the flow status of a given hourly time step forecast from a given NWP. The different lead times of the NWP are aggregated in the results.

Deleted: , which sum up to n

Table 2 displays the verification measures used in this paper, a comprehensive review and further description of verification measures can be found in the meteorological literature, e.g. (WWRP/WGNE, 2009) and (Wilks, 2011).

The probability of detection (PoD) is defined as the fraction of occurrences of events that were correctly forecast (i.e. hits), while the probability of false detection ($PoFD$) is the fraction of non-occurrences of events that were incorrectly forecast (i.e. false alarms). The empirical occurrence frequency (μ) expresses climatological information about the occurrence of events.

Deleted: ed

Deleted: ed

3.2 Brier skill score

The Brier Score (Brier, 1950) assesses forecast quality of discrete probability forecasts predicting binary outcomes (i.e. “events” and “non-events”) and is comparable to the mean square error. For a given t^{th} hourly forecast time step, the forecast probability of an event ($0 \leq f_{EM,t} \leq 1$) is compared to the observation (y_t). If the t^{th} observation is an event (or non-event) then $y_t = 1$ (or $y_t = 0$).

Deleted: ed

$$BS = \frac{1}{n} \sum_{t=1}^n (f_{EM,t} - y_t)^2 \quad (1)$$

The Brier Skill Score (BSS) is formulated as a skill score related to a reference forecast, e.g. climatology in meteorology. In our case the reference forecast is based on the frequency of occurrence of events during the recorded forecast period (μ). A positive value of the BSS indicates that forecast is beneficial compared to the reference forecast.

$$BSS = 1 - \frac{BS}{BS_{ref}} \quad \text{with} \quad BS_{ref} = \frac{1}{n} \sum_{t=1}^n (\mu - y_t)^2 \quad (2)$$

3.3 Relative Operating Characteristic (ROC)

The Relative Operating Characteristic (ROC), which originates from signal detection theory (Mason, 1982), measures the discrimination ability (i.e. the ability to discriminate events and non-events) of an EPS. The ROC plots the PoD versus the $PoFD$ using a set of decreasing probability decision thresholds (Figure 4). The selection of a lower decision threshold f_{EM} to convert the ensemble forecast to a single forecast is more conservative towards correctly predicting events. Therefore the PoD will be higher but the $PoFD$ will increase as well.

The ROC diagram of the flow domain distinction using the weighted areal overlap NWP post-processing method is displayed on Figure 4. The blue dots represent the discrimination skill of each individual ensemble member. Figure 4 shows that all ensemble members have comparable discrimination skill. The red dots correspond to the discrimination skills from all decision thresholds, from $f_{EM} = 1$ at the bottom left (i.e. all ensemble members should agree on the event occurrence) to $f_{EM} = \frac{1}{N}$ on the top right (i.e. the prediction of an event from a single ensemble member is enough to consider an occurrence). Figure 4 underlines that EPS and decision thresholds provide a larger range of available prediction skills than the ensemble member individually. The choice of a decision threshold represents a trade-off between predicting events correctly and generating false alarms.

The skill score of a ROC diagram is calculated based on the area under the curve ($ROCA$). The $ROCA$ ranges from 0 to 1, a score of 1 corresponds to a perfect forecast and a score of 0.5 corresponds to the skill of a random forecast based on the probability of occurrence (μ).

3.4 Relative Economic Value (REV)

A proper evaluation of the benefits of a forecast system should not only consider the forecasts skill e.g. using *PoD* and *PoFD*, or *BSS*. A detailed knowledge of the decision-making process is needed to answer the question: “how does this skill translate to an economic value of a forecast?”. Furthermore when using ensemble forecasts the following question should be answered as well: “which decision threshold and NWP post-processing method for the EPS is the most beneficial for my purpose?”.

The economic benefit from a forecast depends on the alternative courses of action and their consequences. Each course of action is associated with a cost and leads to economic benefit or loss depending on the observed outcome. The task is thus to choose the appropriate actions which will maximize the expected gain or minimize the expected loss. The usefulness of the forecast can thus be quantified by considering the occasions when the forecast was beneficial, detrimental or neutral with respect to the process of decision making.

The relative economic value of our urban hydrological prediction system is here inspired by the relatively simple cost-loss ratio decision model introduced by (Richardson, 2000). Richardson developed this approach to assess the economic value of taking costly actions to mitigate the consequences of forecast adverse weather events in order to reduce the potential loss associated with them. The decision threshold that can empirically be shown to lead to the lowest expense on the long term should be adopted. Richardson illustrated his approach for the problem of roads gritting to prevent the formation of ice. Subsequently Roulin (2006) used this approach to investigate the benefit of river flow mitigation measures for two catchments in Belgium and (Chang et al., 2015) applied it to assess the relevance of typhoon mitigation measures in Taiwan.

All these studies consider adverse events which can be mitigated at a cost, reducing the loss associated with these events, and their decision models are therefore based on a cost-loss ratio. This study investigates a different perspective. Instead of taking mitigating measures when adverse events are predicted, the system is optimised when no events are predicted in order to achieve a positive gain, and left under its traditional management when events are predicted. Therefore our decision model is based on a gain-loss ratio. During low flow periods, when no events are forecast, the management objective is switched to energy consumption by utilising the Smart Grid energy market leading to a gain (G). As a consequence mis-predicted high flow events will jeopardise the IUDWS, e.g. the detention basins may not be empty in time. These negative outcomes are represented by a loss (L). In case of forecast events (hits and false alarms) the management objectives of the IUDWS remain unchanged. The economic outcome of these two situations remains the same therefore a null value is assigned to them, Table 3.

Furthermore Richardson (2000) used a static ratio, the cost of mitigation measures and reduction of loss associated were fixed. This study encompasses the possibility of a time dependent gain-loss ratio. Indeed, the gain (G) from switching the management objectives to energy optimisation depends on the state of the energy market at the given time. Similarly the loss (L) resulting from miss predicted events is related to the current status of the IUDWS, e.g. the volume of water stored.

Based on

Table 2 and Table 3 the expected economic value of using the forecast for decision making over one time step (n represents the total number of time steps) can be expressed empirically as:

$$E_{forecast} = \frac{d \cdot G - c \cdot L}{n} \quad (3)$$

In case of a perfect forecast ($b = c = 0$) the economic value would be:

$$E_{perfect} = d \cdot \frac{G}{n} = (1 - \mu) \cdot G \quad (4)$$

If no forecasts are available, the optimal course of action can be determined based on the empirical frequency of occurrence of an event, μ (climatological information in case of weather event as for (Richardson, 2000)). The two possible courses of

Deleted: on

Deleted: ed

Deleted: optimized

Deleted: ed

Deleted: s

Deleted: ed

Deleted: dynamic,

action are either to always optimise the system despite the losses or to never optimise the system. $E_{statistic}$ considers the highest economic value between these two courses of action (Eq. 4); never optimizing (i.e. the IUDWS management is unchanged) would lead to a null economic value whereas always optimizing would lead to a gain G associated to a loss L when events do occur.

Deleted: optimize

Deleted: optimize

$$5 \quad E_{statistic} = \max(G - \mu * L, 0) \quad (5)$$

The Relative Economic Value (REV), as defined by (Richardson, 2000), compares the benefit of acting on a given forecast to the benefit which would be achieved by acting on a perfect forecast as a ratio (Eq. 5).

$$REV = \frac{E_{forecast} - E_{statistic}}{E_{perfect} - E_{statistic}} \quad (6)$$

The REV expressed by Eq. 6 can be reformulated using Eq. 3, Eq. 4 and Eq. 5 and expressed as a function of the PoD , the $PoFD$, the frequency of occurrence (μ) and the gain-loss ratio ($\alpha = \frac{G}{L}$) as shown by Eq. 7 and displayed on Figure 5.

$$REV = \frac{\alpha * (1 - \mu) * (1 - PoFD) - (1 - PoD) * \mu - \max(\alpha - \mu, 0)}{\alpha * (1 - \mu) - \max(\alpha - \mu, 0)} \quad (7)$$

The possible value of the REV ranges from 1, corresponding to a perfect forecast, to minus infinity. In case of positive REV the use of the forecast is beneficial, whereas a negative REV indicates that using statistical information and either always or never optimising the IUDWS yields a better economic value than using the weather forecast. Hence the REV can be divided in 3 domains: (i) the interval on the right of the curve in which it is preferable to always optimise (dotted domain on the right side of Figure 5), (ii) the interval with positive REV covered by the curve in which using the forecast is beneficial (middle domain on Figure 5) and (iii) the interval on the left in which it is preferable to never optimise (crosshatched domain on the left side of Figure 5). Assuming that a perfect knowledge of the future yields a benefit β (compared to purely statistical information), then using the actual forecast provides a benefit to the user of $(100 * REV) \%$ of β .

Deleted: in

Figure 6 displays the ROC diagram and the REV - α relationship for flow forecast based on the catchment weighted areal overlap post-processing method. As explained in Sect 3.3. the ROC diagram describes the EPS forecast discrimination skill for the different decision thresholds, f_{EM} . To support decision making the ROC diagram is converted to the REV - α relationship. Each point of the ROC diagram (Figure 6a) represents a discrimination skill (PoD , $PoFD$) for a given decision threshold based on the fraction of ensemble members predicting an event (f_{EM}). For each of these points the REV can be determined as a function of the gain-loss ratio α (Eq. 7 and Figure 5).

Deleted: The curves on Figure 6b show the REV - α relationship for the decision thresholds (f_{EM}) highlighted in Fig. 6a. The REV is thus closely related to the ROC as indicated by (Richardson, 2000; Zhu et al., 2002).¶

The green dot (legend 5) on Figure 6a corresponds to a decision threshold $f_{EM} = 1/25$ and provides the highest PoD for this EPS; the REV associated with it, i.e. the green line (legend 5) on Figure 6b, leads to the highest REV for low α values (below 0.105) which corresponds to high a negative impact of missed events. Other decision thresholds yield better REV for higher α , e.g. the decision threshold $f_{EM} = 5/25$ corresponding to the red dot (legend 4) on Figure 6a provides the highest REV (legend 4) for α within the range [0.16; 0.18]. Hence as demonstrated by Richardson (2000) the ensemble has better discrimination and can provide higher REV to a wider range of users (i.e. larger interval with positive REV) than any individual deterministic forecast (colour line) as illustrated by the envelope curve.

4 Results and discussion

4.1 ROC, REV and NWP post-processing methods.

The REV is closely related to the ROC diagram as indicated by (Richardson, 2000; Zhu et al., 2002) and illustrated on Figure 6. The curves on Figure 6b show the REV - α relationship for the decision thresholds (f_{EM}) highlighted in Figure 6a. The green dot (number 5) on Figure 6a corresponds to a decision threshold $f_{EM} = 1/25$ and provides the highest PoD for this EPS; the REV associated with it, i.e. the green line (number 5) on Figure 6b, leads to the highest REV for low α values (below 0.105) which corresponds to a high negative impact of missed events. Other decision thresholds yield better REV for higher α , e.g. the decision threshold $f_{EM} = 5/25$ corresponding to the red dot (legend 4) on Figure 6a provides the highest REV (legend 4) for α within the range [0.16; 0.18]. Hence as demonstrated by Richardson (2000) the ensemble has better discrimination and can provide higher REV to a wider range of users (i.e. larger interval with positive REV) than any individual deterministic forecast (colour line) as illustrated by the envelope curve.

The implementation of the IUDWS energy consumption optimisation scheme is challenged by potentially missed high flow events. Indeed, these situations would lead to inappropriate management, jeopardizing the performance of the IUDWS. As explained in Sect. 2.2, post-processing methods can be applied to enhance the NWP, e.g. by accounting for potentially misplaced events which can have significant impact at an urban hydrology scale. Figure 7 displays the result considering the NWP maximal threat post-processing EPS method with a 6 grid cells radius around the catchment. This approach is more conservative towards avoiding missed events and yields higher PoD at the cost of higher $PoFD$, which extends the ROC diagram. The ROC curves on Figure 7a show that the two approaches are complementary; the areal overlap method provides better discrimination skill for low $PoFD$ whereas the maximal threat EPS post-processing method provides better discrimination skill for higher $PoFD$. The ROCA of each approach is respectively 0.86 and 0.91 and the ROCA merging both approaches is 0.92.

This new ROC curve results in the extension of the α -interval with positive REV which characterises the range of beneficial forecast use (Figure 7b). To ease the comparison the area under the envelop curve of the areal overlap approach is displayed in grey colour as background on Figure 7b, and Table 4 gives intervals of positive α for both approaches. The weighted areal overlap provides a slightly better upper bound whereas the maximal threat approach significantly expands the interval of positive REV for low α values. Therefore, using this NWP post-processing approach increases the range of beneficial forecast usages.

The comparison between these two NWP-post processing approaches using the Brier Skill Score (BSS) shows a deterioration of the forecast skill when using the maximal threat approach, which has a negative BSS indicating that the forecast performs worse than the reference forecast based on the frequency of occurrence of an event (μ). This decrease in performance can be explained by an increase in false alarms due to the precautions towards not missing a major rain event of this approach. This result underlines the need for an economical assessment rather than purely forecast skills to draw conclusions of the usefulness of a forecast for a given decision making situation.

Deleted: that

4.2 Examples of EPS flow domain prediction

In order to illustrate the different situations of decision making taken as a starting point for this paper (i.e. when to switch from flow management to energy management and vice versa) a range of 4 theoretical α -values were considered, Table 5. The two outer α -values yield negative REV indicating that using the forecast data is not beneficial in these cases. The two other α -values yield positive REV indicating that using the forecast is beneficial in these cases. The decision threshold (f_{EM}) generating the highest relative benefit based on empirical data are displayed on Figure 8 and in Table 5.

The coupled hydro-meteorological model provides an ensemble prediction of the flow at the catchment outlet for the incoming 2 days. Figure 9 provides an example of prediction. The first panel, Figure 9a, displays the energy market during those two days, providing insight in the variation of the energy price and the CO₂ footprint through the proportion of wind energy. The shown data are based on historical values but similar information are available in real time on the electric smart grid. The fluctuation of the energy market for both parameters (Figure 9a) illustrates the variation of the α -value in relation to the potential gain during a given period. During the first day (29th April 2015) the energy price ranges from 24 €/MWh to 32 €/MWh and the proportion of wind energy varies from 15 % to 49 %, whereas during the second day (30th April 2015) the energy price range from 23 €/MWh to 41 €/MWh and the proportion of wind energy varies from 1 % to above 53 %. Hence the switch of consumption of 1 MWh can yield up to 8 € during the first day and up to 18 € during the second day. For comparison, the energy consumption per m³ treated at Damusåen WWTP in 2015 was 0.261 kWh/m³ and in average 20,000 m³ are treated during a dry day. Pumping and aeration of the biological treatment are the dominating energy users. The aeration of the bioreactor represents between 50 and 70 % of process energy consumption and largely depends on the inflow/load to the WWTP (Aymerich et al., 2015). The potential for energy switch highly depends to the storage volume available upstream.

Deleted: forecasted by

Deleted: and available in real time

The North Pool Energy Market DK2, covering the Copenhagen area, has a Pearson correlation coefficient of -0.52 between energy price and proportion of wind energy in 2015, indicating a moderate negative linear relationship. Hence energy consumption optimisations based on economic objectives could also yield environmental benefits and vice versa. However it should be noticed that the control of the energy consumption based on the energy market can result in a decrease of the expenses together with an increase of the overall energy consumption as observed in (Aymerich et al., 2015).

Deleted: Furthermore energy consumption optimisation based on economic objectives will also yield environmental benefits and vice versa. Indeed the energy price and the proportion of wind energy are negatively correlated.

Deleted: e.g.

Figure 9b represents the flow forecast based on the catchment weighted areal overlap approach and Figure 9c represents the flow forecast based on the maximal threat EPS approach with a 6 grid cells radius. The measured flow during this period shows two minor rain events without significant flow impact the first day and a major rain event leading to high flows exceeding the 4,000 m³ in the IUDWS the second day. Figure 9b illustrates the difficulty of the prediction to have a correct timing, most EMs predict the high flow event but often too early. It can be noticed that due to the conservativeness of this second approach the EPS plume of flow forecasts overestimates the observed flow (in red), which explains the worsening of the BSS when using this approach.

Deleted:

The best flow domain predictions, considering a given α , is provided by the decision threshold defined using the REV method presented in Sect. 3.4. As displayed in Table 5, the highest REV for $\alpha=1/20$ (respectively $\alpha=1/100$) is achieved using the NWP post-processing approach “Maximal Threat EPS” with $f_{EM} = \frac{11}{25}$ (respectively $f_{EM} = \frac{1}{25}$). The flow domain predictions based on these criteria and on the EPS flow forecast displayed on Figure 9b and Figure 9c are shown by the blue hatched (respectively plain blue) colour in Figure 9d.

4.3 Outlooks

As mentioned in the previous Sect. 4.2, the potential benefit from the energy consumption optimisation management is largely conditioned by the storage volume available upstream. A major project is currently under implementation to comply with new regulations on CSO. Two large pipes will be constructed just before the inlet of the WWTP with a volume equivalent to the daily dry weather flow to the WWTP. This large storage volume soon available upstream the WWTP provides an opportunity for real world implementation of the concept developed in this paper. (Halvgaard et al., submitted 2017) presents a Model Predictive Control (MPC) to control the power consumption of pumps in a sewer system and the treatment power consumption according to electricity prices and effluent quality (nitrogen) based on a case study at Kolding. The controller is able to balance electricity costs and treatment quality during predicted dry weather flow periods.

The predictions and therefore the skills of the EPS are based on a coupled meteorological and hydraulic model. This study used a lumped conceptual hydraulic model; a more detailed hydrological model including stochastic processes and on-line assimilation of flow measurements might improve the prediction and thereby improve the REV further. Similarly, NWP models are continuously improving and benefit from the constant increase of computational calculation power to enhance their resolution and ensemble size. The techniques of data assimilation from radar measurement into NWP models are also consistently improving (Korsholm et al., 2015). Weather services are collaborating to continuously improve their meteorological models. The HIRLAM consortium which developed the model structure of the DMI-HIRLAM-S05 NWP used in this study is e.g. currently developing and launching the non-hydrostatic convection-permitting HARMONIE model in cooperation with Météo-France and ALADIN, and EPS with forecast horizons of up to two weeks are also available at the European level (<http://www.ecmwf.int/>). Therefore the accuracy and lead time of the prediction and hence the potential benefit from the framework developed in this article is expected to increase in the future.

Additionally, other characteristic of NWP can be utilised. The DMI-HIRLAM-S05 model e.g. generates a new 54 h EPS forecast every 6 hours, and thereby the successive forecasts are overlapping each other. The forecast consistency, or in reverse the “forecast jump”, provides valuable information on forecast uncertainty which could be utilised in the decision making process. For example the time-lagged method (Mittermaier, 2007) uses consecutive forecast overlapping to extend the EPS and enhance the predictions (i.e. the horizon of the forecast is reduced but its ensemble size is increased). This may

increase the range of positive *REV* and allow use of the concept for decisions related to other problems than the energy optimization problem studied here.

Control systems can be decomposed into different layers in a hierarchy. Mollerup et al. (2016) presents a methodological approach to the design of optimising control strategies for sewer systems. The framework presented in this paper targets the upper layer of the hierarchy presented by Mollerup et al. (2016): the management of objectives where switching between different operational modes may take place. Completely different optimising control strategies, including model predictive control techniques, may then run under different operation conditions – such as the “flow control” and “energy optimisation” operational modes considered in this paper. Implementing such a switching system in practice requires that the gain/loss ratio expressing the economic consequences associated with the outcomes of the different course of actions used for the *REV* is quantified, which requires further research on monetization of non-market goods, e.g. CO₂ footprint or the environmental impact of CSOs, and may depend on local circumstances.

5 Conclusion

An ensemble flow prediction system for an IUDWS was developed using the DMI-HIRLAM-S05 EPS as input to a hydrological model. This system was tested on an urban catchment in the Copenhagen area based on recorded rainfall forecasts and flow data for the period from June 2014 to May 2016. Ensemble forecasting requires adapting the management rules in order to use probability forecasts instead of a deterministic forecast. The usefulness of the forecast should be evaluated not only based on its quality in terms of traditional skill scores but also based on its economic value for the daily decision-making process of the forecast user considered. The decision problem considered here is the switching from normal flow management during high flow periods (wet weather) to Smart Grid energy optimization during low flow periods (dry weather).

This article presents a framework to support decision making based on the prediction of the occurrence or no occurrence of an event using an ensemble predicting system (EPS). The outcomes (gain for positives and loss for negatives) of the different possible courses of action are valued to determine the Relative Economical Value (*REV*) of using the forecast. The *REV* is closely related to the ROC diagram, which assesses the range of discrimination skills of an ensemble forecast. Hence a *REV* curve, as a function of the gain/loss ratio α , can be generated for each probability threshold (f_{EM}) of the EPS. This method was developed in order to switch the IUDWS management objective from flow management to energy optimization utilising the electric Smart Grid when low flow periods are predicted. This approach is based on daily optimisation when non-events (dry weather) are forecast and differs from previous studies based in the *REV* concept which investigated mitigation measures taking place when adverse events are forecast (e.g. flood, tornado) using a cost/loss ratio. In our approach for a given gain-loss ratio α , the probability threshold (f_{EM}) corresponding to the highest *REV*, symbolised by the envelop curve, should be applied to maximize the benefit of the optimisation scheme. If the gain-loss ratio is outside the range of positive *REV*, then using the forecast is not beneficial. The gain-loss ratio α is function of the potential gain from utilising the variation of the Smart Grid energy market which varies in time.

Two NWP post-processing methods were tested: (i) a realistic approach based on the weighted areal overlap between the NWP grid cells and the hydrological catchment and (ii) a more conservative approach considering the maximal rainfall threat in the catchment vicinity. The second approach leads to a deterioration of classic forecast validation scores such as Brier Skill Score due to a significant increase in the number of false alarms. However, this approach proves to be beneficial in regard to the decision making process especially when considering a low gain-loss ratio α for which missed forecast events are highly detrimental. Indeed, the maximal threat NWP neighbourhood post-processing method improves the range of discrimination skill of the predictions shown on ROC diagram and therefore provides a larger range of positive *REV*,

Deleted: ed

Deleted: ed

Deleted: dynamic and depends e.g. on

Deleted: at a given point

Deleted: ed

increasing the range of beneficial forecast usage. This underscores the importance of assessing the forecast usefulness based on its potential economic value rather than solely on the usual forecast skills.

Deleted: is

Deleted: g

Acknowledgment

This research was financially supported by the industrial PhD programme of the Innovation Fund Denmark. The catchment and flow data were kindly provided by Copenhagen Utility Company (HOFOR). We would like to thank the Danish Meteorological Institute (DMI), especially Henrik Feddersen, for providing EPS data from their NWP model DMI-HIRLAM-S05.

References

- Atger, F.: Verification of intense precipitation forecasts from single models and ensemble prediction systems, *Nonlinear Process. Geophys.*, 8(6), 401–417, doi:10.5194/npg-8-401-2001, 2001.
- Aymerich, I., Rieger, L., Sobhani, R., Rosso, D. and Corominas, L.: The difference between energy consumption and energy cost: Modelling energy tariff structures for water resource recovery facilities, *Water Res.*, 81, 113–123, doi:10.1016/j.watres.2015.04.033, 2015.
- Bacher, P., Madsen, H. and Nielsen, H. A.: Online short-term solar power forecasting, *Sol. Energy*, 83(10), 1772–1783, doi:10.1016/j.solener.2009.05.016, 2009.
- BIOFOS: Miljøberetning, Copenhagen. [online] Available from: <http://www.biofos.dk/wp-content/uploads/2014/11/Miljoeberetning-2015.pdf>, 2015.
- Bjerg, J. E., Grum, M., Courdent, V., Halvgaard, R., Vezzaro, L. and Mikkelsen: Coupling of Weather Forecasts and Smart Grid-Control of Wastewater inlet to Kolding WWTP (Denmark), in 10th International Urban Drainage Modelling Conference, pp. 47–59, Mont Sainte-Anne, Québec, Canada., 2015.
- Brier, G. W.: Verification of forecasts expressed in terms of probability, *Mon. Weather Rev.*, 78(1), 1–3, doi:10.1175/1520-0493(1950)078<0001:VOFEIT>2.0.CO;2, 1950.
- Chang, H.-L., Yang, S.-C. and Yuan, H.: Analysis of the Relative Operating Characteristic and Economic Value Using the LAPS Ensemble Prediction System in Taiwan, *Mon. Weather Rev.*, 143, 1833–1848, doi:10.1175/MWR-D-14-00189.1, 2015.
- Collischonn, W., Morelli Tucci, C. E., Clarke, R. T., Chou, S. C., Guilhon, L. G., Cataldi, M. and Allasia, D.: Medium-range reservoir inflow predictions based on quantitative precipitation forecasts, *J. Hydrol.*, 344(1–2), 112–122, doi:10.1016/j.jhydrol.2007.06.025, 2007.
- Courdent, V., Grum, M. and Mikkelsen, P. S.: Distinguishing high and low flow domains in urban drainage systems 2 days ahead using numerical weather prediction ensembles, *J. Hydrol.*, doi:http://dx.doi.org/10.1016/j.jhydrol.2016.08.015, 2016.
- Cuo, L., Pagano, T. C. and Wang, Q. J.: A Review of Quantitative Precipitation Forecasts and Their Use in Short- to Medium-Range Streamflow Forecasting, *J. Hydrometeorol.*, 12(5), 713–728, doi:10.1175/2011JHM1347.1, 2011.
- Damrath, U., Doms, G., Frühwald, D., Heise, E., Richter, B. and Steppeler, J.: Operational quantitative precipitation forecasting at the German Weather Service, *J. Hydrol.*, 239(1–4), 260–285, doi:10.1016/S0022-1694(00)00353-X, 2000.
- Du, J.: Uncertainty and Ensemble Forecast. [online] Available from: <http://www.nws.noaa.gov/ost/climate/STIP/STILecture1.pdf>, 2007.
- Feddersen, H.: A Short-Range Limited Area Ensemble Prediction System, Copenhagen. [online] Available from: <http://www.dmi.dk/fileadmin/Rapporter/TR/tr09-14.pdf>, 2009.
- Giebel, G., Badger, J., Landberg, L., Nielsen, H. A., Nielsen, T. S., Madsen, H., Sattler, K., Feddersen, H., Vedel, H., Tøfting, J., Kruse, L. and Voulund, L.: Wind power prediction using ensembles, Roskilde. [online] Available from:

- http://www.risoe.dk/Knowledge_base/publications/Reports/ris-r-1527.aspx?sc_lang=en, 2005.
- Hadjsaid, N. and Sabonnodière, J.-C.: Smart Grids, First., ISTE Ltd, London UK., 2012.
- Halvgaard, R., Vezzaro, L., Mikkelsen, P. S., Grum, M., Munk-Nielsen, T., Tychsen, P. and Madsen, H.: Integrated Model Predictive Control of Wastewater Treatment Plants and Sewer Systems in a Smart Grid, 1–16, *Computers & Chemical Engineering*, Submitted 2017.
- Harremoës, P., Pedersen, C. M., Laustsen, A., Sørensen, S., Laden, B., Friis, K., Andersen, H. K., Linde, J. J., Mikkelsen, P. S. and Jakobsen, C.: Funktionspraksis for afløbssystemer under regn., 2005.
- Jørgensen, H. K., Rosenorn, S., Madsen, H. and Mikkelsen, P. S.: Quality control of rain data used for urban runoff systems, in *Water Science and Technology*, vol. 37, pp. 113–120., 1998.
- Korsholm, U. S., Petersen, C., Sass, B. H., Nielsen, N. W., Jensen, D. G., Olsen, B. T., Gill, R. and Vedel, H.: A new approach for assimilation of 2D radar precipitation in a high-resolution NWP model, *Meteorol. Appl.*, 22(1), 48–59, doi:10.1002/met.1466, 2015.
- Laloy, E. and Vrugt, J. a.: High-dimensional posterior exploration of hydrologic models using multiple-try DREAM (ZS) and high-performance computing, *Water Resour. Res.*, 48(1), 1–18, doi:10.1029/2011WR010608, 2012.
- Langergraber, G., Alex, J., Weissenbacher, N., Woerner, D., Ahnert, M., Frehmann, T., Half, N., Hobus, L., Plattes, M., Spering, V. and Winkler, S.: Generation of diurnal variation for influent data for dynamic simulation, *Water Sci. Technol.*, 57(9), 1483–1486, doi:10.2166/wst.2008.228, 2008.
- Leu, S.-Y., Rosso, D., Larson, L. E. and Stenstrom, M. K.: Real-time aeration efficiency monitoring in the activated sludge process and methods to reduce energy consumption and operating costs, *Water Environ. Res.*, 81(12), 2471–2481, doi:10.2175/106143009X425906, 2009.
- Mason, I.: A model for assessment of weather forecasts, *Aust. Met. Mag.*, 30, 291–303, 1982.
- Mittermaier, M. P.: Improving short-range high-resolution model precipitation forecast skill using time-lagged ensembles, *Q. J. R. Meteorol. Soc.*, 133, 1487–1500, doi:10.1002/qj, 2007.
- Møllerup, A. L., Mikkelsen, P. S. and Sin, G.: A methodological approach to the design of optimising control strategies for sewer systems, *Environ. Model. Softw.*, 83, 103–115, doi:10.1016/j.envsoft.2016.05.004, 2016.
- Nash, S. E.: The Form of the Instantaneous Unit Hydrograph, *IASH Publ.*, 114–121, 1957.
- Pappenberger, F., Scipal, K. and Buizza, R.: Hydrological aspect of meteorological verification, *Atmos. Sci. Lett.*, 9(April), 43–52, doi:10.1002/asl.171, 2008.
- Richardson, D. S.: Skill and relative economic value of the ECMWF ensemble prediction system, *Q. J. R. Meteorol. Soc.*, 126(563), 649–667, 2000.
- Rosso, D. and Stenstrom, M. K.: Comparative economic analysis of the impacts of mean cell retention time and denitrification on aeration systems, *Water Res.*, 39(16), 3773–3780, doi:10.1016/j.watres.2005.07.002, 2005.
- Roulin, E.: Skill and relative economic value of medium-range hydrological ensemble predictions, *Hydrol. Earth Syst. Sci. Discuss.*, 3(4), 1369–1406, doi:10.5194/hessd-3-1369-2006, 2006.
- Shrestha, D. L., Robertson, D. E., Wang, Q. J., Pagano, T. C. and Hapuarachchi, H. a P.: Evaluation of numerical weather prediction model precipitation forecasts for short-term streamflow forecasting purpose, *Hydrol. Earth Syst. Sci.*, 17(5), 1913–1931, doi:10.5194/hess-17-1913-2013, 2013.
- Sun, J., Xue, M., Wilson, J. W., Zawadzki, I., Ballard, S. P., Onvlee-Hooimeyer, J., Joe, P., Barker, D. M., Li, P. W., Golding, B., Xu, M. and Pinto, J.: Use of nwp for nowcasting convective precipitation: Recent progress and challenges, *Bull. Am. Meteorol. Soc.*, 95(3), 409–426, doi:10.1175/BAMS-D-11-00263.1, 2014.
- Theis, S. E., Hense, a and Damrath, U.: Probabilistic precipitation forecasts from a deterministic model: a pragmatic approach, *Meteorol. Appl.*, 12(3), 257, doi:10.1017/S1350482705001763, 2005.
- Uden, P., Rontu, L., Jarvinen, H., Lynch, P., Calvo, J., Cats, G., Cuxart, J., Eerola, K., Fortelius, C., Garcia-moya, J. A.,

Jones, C., Lenderlink, G., Mcdonald, A., Mcgrath, R. and Navascues, B.: HIRLAM-5 Scientific Documentation, Norrköping. [online] Available from: http://hirlam.org/index.php/component/docman/doc_view/270-hirlam-scientific-documentation-december-2002?Itemid=70, 2002.

Weron, R.: Modeling and forecasting electricity loads and prices: A statistical approach, First Edit., John Wiley & Sons Ltd., 2006.

Wilks, D. S.: Statistical Methods in the Atmospheric Sciences, Elsevier., 2011.

WWRP/WGNE: Recommendations for the Verification and Intercomparison of QPFs and PQPFs from Operational NWP Models, Geneva, Switzerland. [online] Available from: http://www.wmo.int/pages/prog/arep/wwrp/new/documents/WWRP2009-1_web_CD.pdf, 2009.

Zhu, Y., Toth, Z., Wobus, R., Richardson, D. and Mylne, K.: The economic value of ensemble-based weather forecasts, Bull. Am. Meteorol. Soc., 83(January), 73–83, 2002.

Zugno, M.: Optimization under uncertainty for management of renewables in electricity markets, University of Denmark. [online] Available from: [http://orbit.dtu.dk/en/publications/optimization-under-uncertainty-for-management-of-renewables-in-electricity-markets\(d314a0c4-185f-4983-95ff-21133defd41d\).html](http://orbit.dtu.dk/en/publications/optimization-under-uncertainty-for-management-of-renewables-in-electricity-markets(d314a0c4-185f-4983-95ff-21133defd41d).html), 2013.

Table 1: Contingency table (with n the sample size)

Event forecast	Event observed		
	Yes	No	
Yes	hits (<i>a</i>)	false alarms (<i>b</i>)	<i>a + b</i>
No	misses (<i>c</i>)	correct negatives (<i>d</i>)	<i>c + d</i>
	<i>a + c</i>	<i>b + d</i>	<i>a + b + c + d = n</i>

Deleted: ed

Table 2: Verification measures based on the contingency table

Score	Formula	Range	Perfect
Probability of detection, <i>PoD</i>	$a/(a + c)$	[0,1]	1
Probability of false detection, <i>PoFD</i>	$b/(b + d)$	[0,1]	0
Occurrence frequency of events, μ	$(a+c)/n$	[0,1]	na

Table 3 : Economical value assigned to the different outcomes of the contingency table (L:loss; G:gain).

Event forecast	Event observed	
	Yes	No
Yes	0	0
No	L	G

Deleted: ed

Table 4: *BSS* and *REV* characteristics for the two different NWP post-processing methods

	<i>ROCA</i>	α -interval		<i>BBS</i>
		Lower bound	Upper bound	
Weighted areal overlap	0.86	0.0208	0.3955	0.14
Maximal threat 6 cells radius	0.91	0.0049	0.3940	-1.52

5 Table 5: Decision threshold and *REV* for the theoretical 4 α -values considered, using the maximal threat post-processing method.

α	<i>REV</i>	Prediction criteria	
		Decision Threshold	NWP post-processing
1/2	Negative	Always <u>energy objective</u>	
1/20	0.59	$f_{EM} = 11/25$	Maximal Treat EPS
1/100	0.30	$f_{EM} = 1/25$	Maximal Treat EPS
1/500	Negative	Never <u>energy objective</u>	

Deleted: optimise

Deleted: optimise

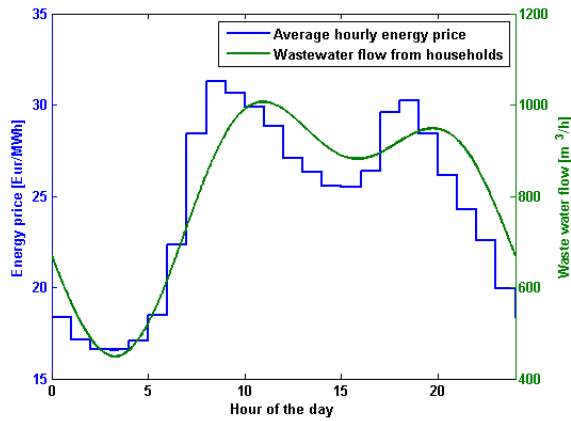


Figure 1: Yearly average (2015) of hourly energy price for the energy market DK2 covering the Copenhagen region (in blue, data from <http://www.nordpoolspot.com/>). Calibrated daily variation of the dry weather flow for the Damhusåen catchment (green) used for demonstration in this paper see further details in Sect. 2.3.

10


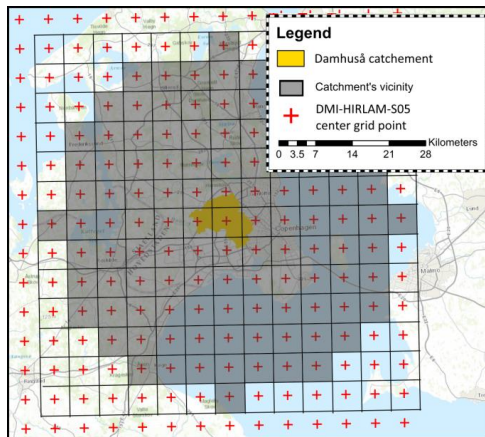


Figure 2: Illustration of the 6 grid cells radius used by the maximal threat neighbourhood approach, for the Damhuså catchment used for demonstration in this paper (Courdent et al., 2016).

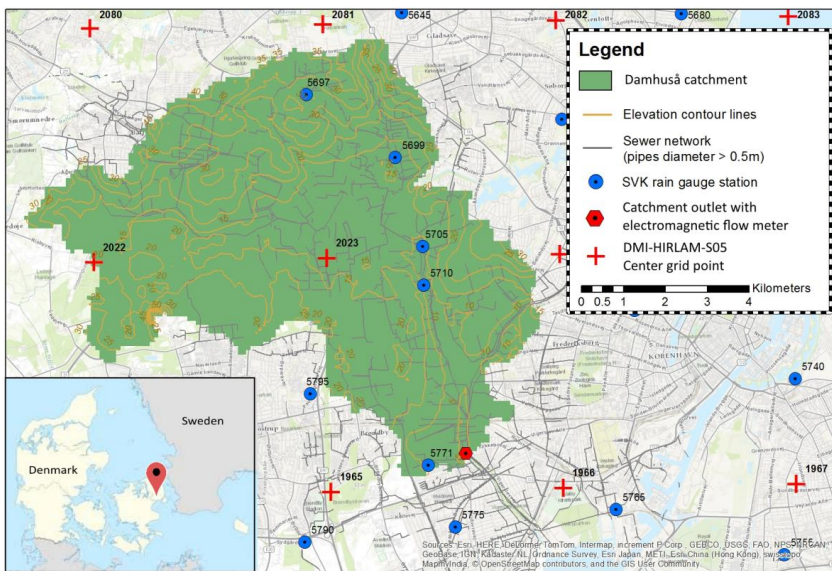

5 | Figure 3: The Damhuså urban drainage catchment, Copenhagen, Denmark (contributing area, green area on the map).

Deleted: , 67 km²

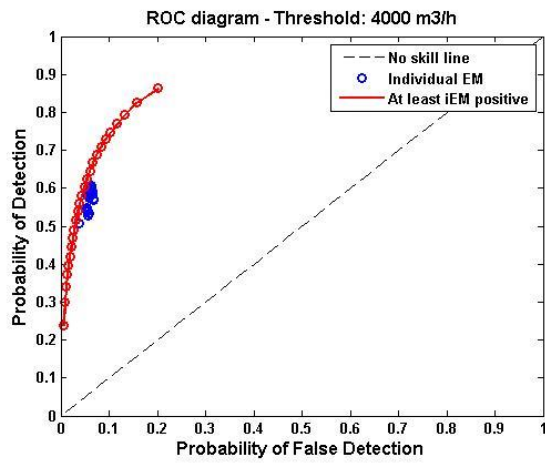


Figure 4: Example of Relative Operating Characteristic (ROC) diagram.

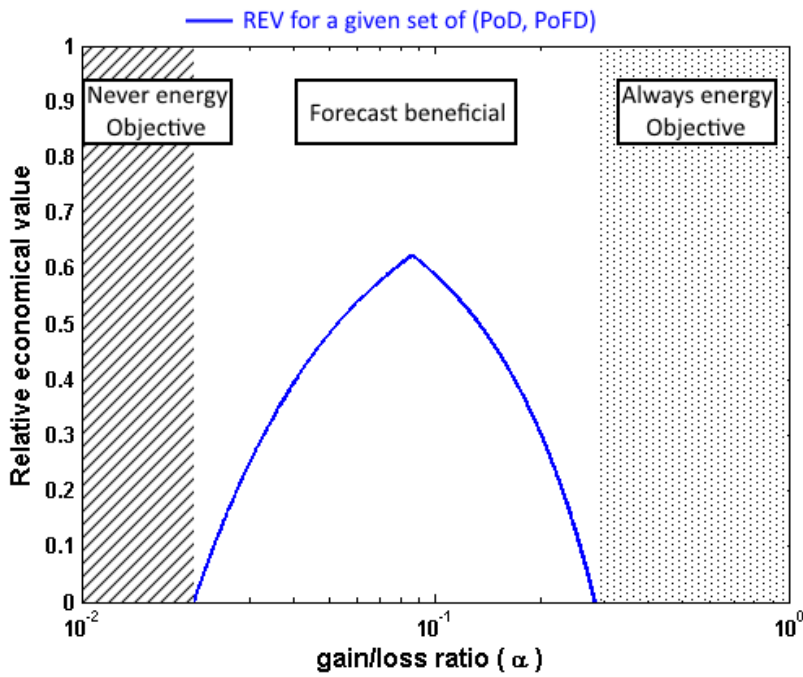


Figure 5: The 3 domains of operation of the REV curve as a function of the gain-loss ratio α .

Comment [VATC1]: New figure – “Never optimized” replaced by “Never energy objective”
 “Always optimized” replaced by “Always energy objective”


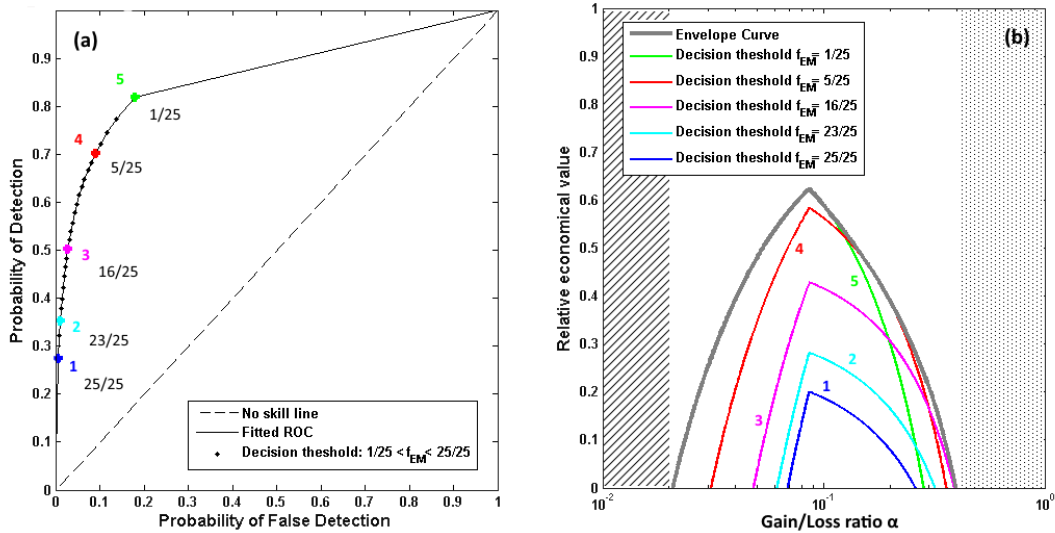


Figure 6: ROC and REV diagram for flow domain forecast based on catchment weighted areal overlap.

Comment [VATC2]: New figure.

Correction in the legend, change in location of the number (3, 4, 5).

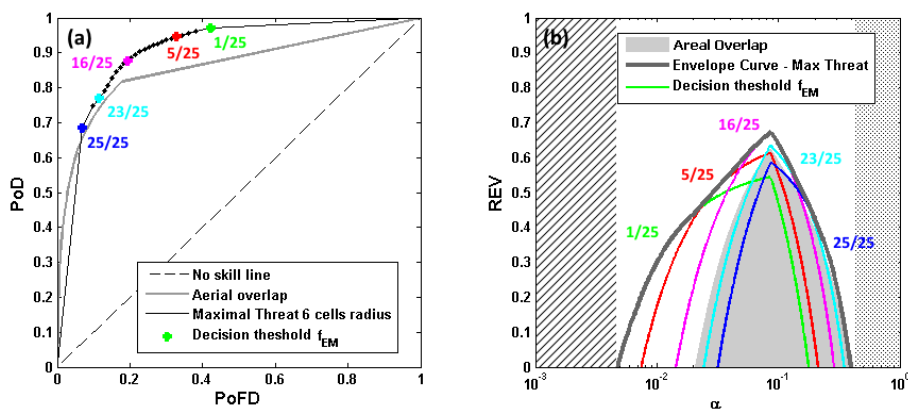

5 Figure 7: ROC and REV diagram for flow forecasts considering the two NWP post-processing methods: The maximal threat EPS method with a neighbourhood radius of 6 grid cells in colour and the catchment weighted areal overlap method in grey colour as background.

Comment [VATC3]: New figure.

Correct typo in legend

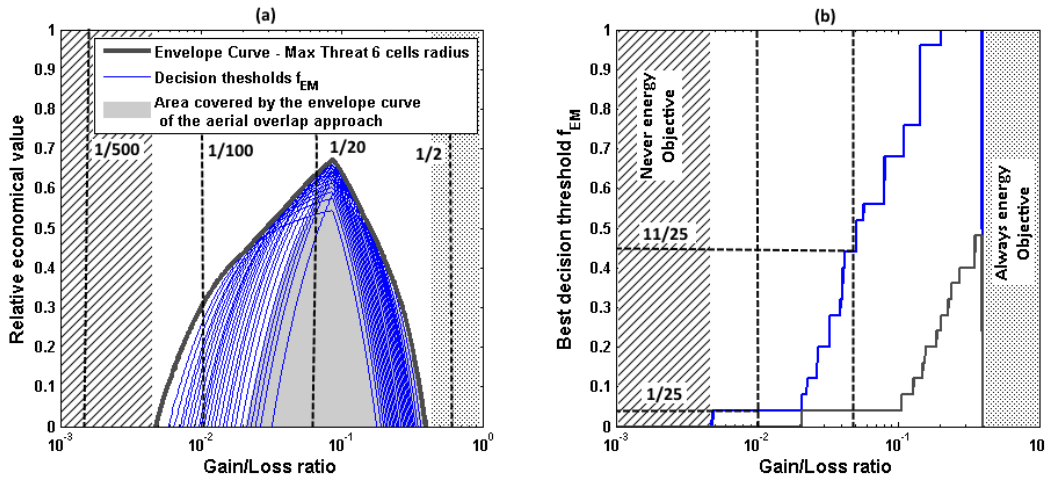


Figure 8: REV curves for the EPS NWP post-processing maximal threat in a radius of 6 grid cells from the catchment (a, left plot) and best decision threshold according to the α -value (b, right plot), in blue for the maximal threshold approach and in grey for the aerial overlap approach.

Comment [VATC4]: New figure

“Never optimized” replaced by “Never energy objective”
 “Always optimized” replaced by “Always energy objective”

5

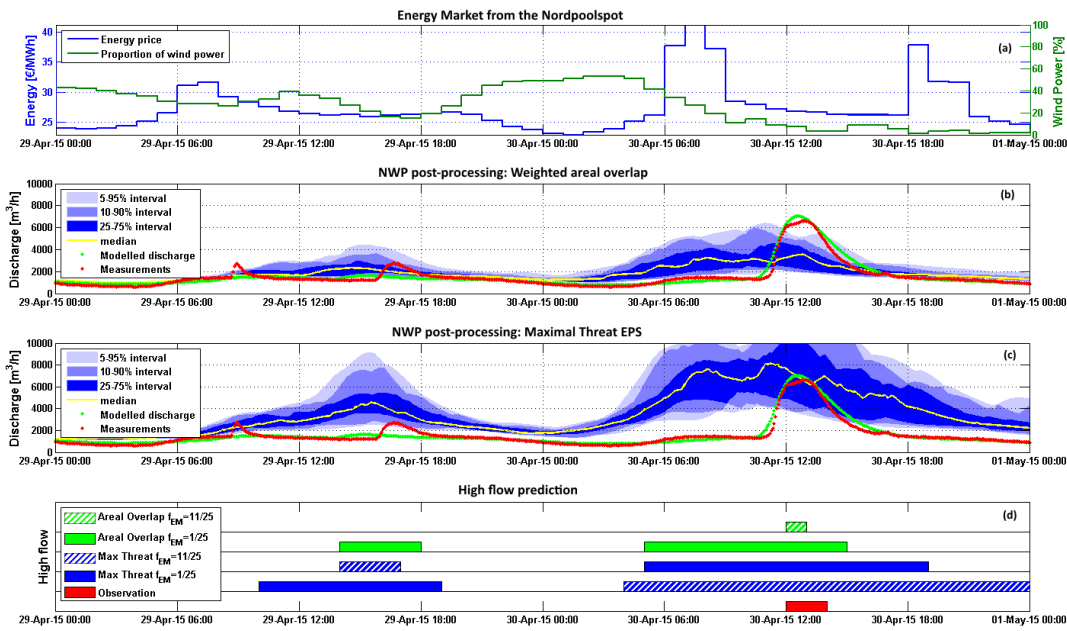


Figure 9: Example illustration of the EPS flow prediction system for two selected days, 29-30 April 2015. Energy market parameters, energy price and proportion of wind power (1, top plot), ensemble flow predictions using the areal average (b) and maximal threat (c) post-processing methods, and (d) flow domain predictions for the two post-processing methods and for each two decisions thresholds, cf. Table 5 (coloured areas imply that an event is predicted, otherwise not).

Comment [VATC5]: New figure with legend in (a) and modelled discharge from rainfall measurement.

10