

Technical note: A new laboratory approach to extract soil water for stable isotope analysis from large soil samples

Jiri Kocum^{1,2}, Jan Haidl¹, Ondrej Gebousky¹, Kristyna Falatkova¹, Vaclav Sipek¹, Martin Sanda³, Natalie Orłowski⁴, and Lukas Vlcek¹

5

¹ Institute of Hydrodynamics of the Czech Academy of Sciences, Prague, 160 00, Czech Republic

² ~~Faculty of Science~~, Department of Physical Geography and Geocology, ~~Faculty of Science~~, Charles University, Prague, 128 00, Czech Republic

³ ~~Faculty of Civil Engineering~~, Department of Landscape Water Conservation, ~~Faculty of Civil Engineering~~, Czech Technical University, Prague, 166 29, Czech Republic

10

⁴ ~~Chair of Forest Sites and Hydrology~~, Institute of Soil Science and Site Ecology, ~~Chair of Forest Sites and Hydrology~~, Technical University Dresden, Tharandt, 01737, Germany

Correspondence to: Jiri Kocum (kocum@ih.cas.cz)

15

Abstract. A correct soil water extraction represents an initial step in stable water isotope analysis. To this aim, we present a new soil water extraction method based on the principle of complete evaporation and condensation of the soil water in a closed circuit. The proposed device has four extraction slots and can be used up to two times a day. Owing to its simple design, there is no need for any chemicals, gases, high pressure or high-temperature regimes. The experimental tests proved that the extraction itself does not cause any major isotope fractionation effects leading to erroneous results. Extraction of pure water samples shifts the isotope composition by 0.04 ± 0.06 ‰ and 0.06 ± 0.35 ‰ for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively. Soil water extraction tests were conducted with five distinct soil types (loamy sand, sandy loam, sandy clay, silt loam, and clay) using 40-150 grams of pre-oven-dried soil, which was subsequently rehydrated to 10 and 20 % water content. The shift in the isotopic composition of these tests ranged between -0.04 and 0.07 ‰ for $\delta^{18}\text{O}$ and 0.4 and 1.3 ‰ for $\delta^2\text{H}$ with the standard deviation of $\pm (0.08 - 0.25)$ ‰ and $\pm (0.34 - 0.58)$ ‰ for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively. The results exhibit high accuracy which makes this method suitable for high-precision studies where unambiguous determination of the water origin is required.

20

25

1 Introduction

Measurements of soil water isotopic composition (^2H and ^{18}O) provide a description of soil water movement and mixing processes in the vadose zone (Stumpp et al., 2018). In some cases, different trends in soil water samples characterisation without an application of exact isotopic composition method (tracer experiments to prove interconnection) give a sufficient information about samples dissimilarity. However, for characterizing the transport processes and residence time, accurate evaluation of sample origin, soil water dynamics modelling or inter-laboratory comparison, the exact values of the isotopic composition are indispensable. This justifies an emphasis paid to correct soil water extraction. Unlike liquid water samples of

30

precipitation, snow cover, stream or groundwater, where the isotopic compositions are easily accessible, the extraction of matrix- or tightly-bound soil water is challenging from the viewpoint of exact determination of isotopic composition. It has
35 been shown that the storage and sample preparation for extraction, soil texture, soil water content as well as organic matter and carbonate content strongly influence the final results (West et al., 2006; Wassenaar et al., 2008; Koeniger et al., 2011; Meißner et al., 2014; Hendry et al., 2015; Orłowski et al., 2016a; Newberry et al., 2017). Parallely, the specifics of extraction methods, e.g., the different pore spaces that may or may not be extracted via the different approaches (Orłowski et al., 2019; Kübert et al., 2020) and the modifications of the procedures themselves (Orłowski et al., 2018) can affect the isotope results.

40 There are several classes of different extraction methods, some of them were compared in Zhu et al. (2014); Sprenger et al. (2015); and Orłowski et al. (2016b, 2018). In brief, there are the methods using

- a) various chemical compounds or elements like toluene for azeotropic distillation (Revesz and Woods, 1990; Thorburn et al., 1993), dichloromethane for accelerated solvent extraction techniques (Zhu et al., 2014), zinc or uranium for microdistillation (Kendall and Coplen, 1985; Brumsack et al., 1992);
- 45 b) microwave water extraction (Munksgard et al., 2014);
- c) force in terms of mechanical squeezing (Wershaw et al., 1966; White et al., 1985; Böttcher et al., 1997) or centrifugation (Mubarak and Olsen, 1976; Batley and Giles, 1979; Barrow and Whelan, 1980; Peters and Yakir, 2008);
- d) equilibration methods such as in situ equilibration (Garvelmann et al., 2012; Rothfuss et al., 2013, 2015; Volkmann and Weiler, 2014; Gaj et al., 2016), CO₂- and H₂-equilibration (Jusserand, 1980; Scrimgeour, 1995; Hsieh et al., 1998;
50 McConville et al., 1999; Koehler et al., 2000; Kelln et al., 2001) and the direct liquid-vapour equilibrium laser spectroscopy (DVE-LS) method (Wassenaar et al., 2008; Hendry et al., 2015);
- e) cryogenic vacuum extraction (CVE) (Dalton, 1988; West et al., 2006; Koeniger et al., 2011; Goebel and Lascano, 2012; Orłowski et al., 2013, 2016; Gaj et al., 2017), modified CVE – He-purging method (Ignatev et al., 2013) and automatic cryogenic vacuum distillation (ACVD) system LI-2100 (Lica United Technology Limited Inc.).

55 In addition, many laboratories use various modifications of these methods (Walker et al., 1994; Munksgaard et al., 2014; Orłowski et al., 2018). A more detailed description of the above-stated methods is presented in Sprenger et al. (2015) and Ceperley et al. (2024).

At present, the DVE-LS and CVE are the most commonly used methods for soil water extraction. Both methods provide very accurate results, but only under specific conditions. For the DVE-LS method, the different equilibration times,
60 low water content as well as the selection of bags play a crucial role (Hendry et al., 2015; Gralher et al., 2016). It has been also shown that soil samples with a high content of fine particles, thus high soil tension, can cause isotope fractionation in closed systems (Gaj and McDonnell, 2019). For the CVE method, the major challenge is the treatment of soils containing clay minerals. Such soils require application of higher temperatures (up to 300 °C). However, this results in releasing water by oxidation of organics and dihydroxylation of hydroxide-containing minerals such as goethite (Gaj et al., 2017), and in such a way in
65 affecting the experimental results. Moreover, the soil sample size acceptable for this method is rather low, usually between 10 to 20 grams, allowing for the extraction of only grams of the soil water. Another disadvantage of the CVE method consists in

incomparable outputs among different laboratories due to the CVE setup modifications and different workflows (Orlowski et al., 2018). Laboratories' differences in their setups are: the extraction containers (form, size, volume, and material), the heating module and its working temperature (heating tapes or lamps, water baths or hot plates), the type of fittings and connections
70 (glass, stainless steel), and the vacuum-producing units. In addition, different temperatures, pressures, extraction times and sample sizes are applied by different laboratories. However, if a certain setup of all these parameters for the given situation is chosen, very accurate results can be achieved for certain soil types and water contents. Nevertheless, each of these two methods exhibits apparent inconvenience:

- in the case of the DVE-LS method, significant time consumption (a requirement of the permanent presence of an operator);
- 75 - in the case of the CVE method an application of technically complicated methods (work with liquid nitrogen, low pressures and high temperatures in an open laboratory apparatus).

In this study, we present a new extraction method – Circulating Air Soil Water Extraction (CASWE). It is a relatively simple inexpensive method handling soil samples of different sizes, moisture contents and textures. It is based on the simple principle of complete evaporation and condensation in a closed circuit and does not require an application of hazardous
80 substances (acids, toluene, liquid nitrogen), high temperatures and pressures. In the following we (1) introduce a new extraction principle, (2) present the results of soil extraction efficiency testing, and (3) compare the results with other state-of-the-art approaches. The advantage of the proposed method over the others is its accuracy, even with clay samples, known for causing inaccurate results for other extraction methods (Ceperley et al., 2024). The biggest advantages of this extraction method are

- a) high accuracy of the results;
- 85 b) simple design and low cost of the apparatus setup;
- c) low operating costs;
- d) time reduction in operating the device;
- e) ability to process large soil samples and thus obtain large and representative quantities of soil water.

2 Methodology

90 2.1 Principle of extraction

The CASWE method is based on the principle of complete evaporation and subsequent condensation of soil water in a closed circuit using air as the circulating medium. The soil sample is heated inside the evaporation chamber to 105 °C, and the evaporated soil water is carried by air circulation to a cooling unit, where the water vapour condenses, and finally, the liquid water is collected. Dried cool air is then circulated back into the evaporation chamber. The process continues until no air
95 moisture condensation is visible.

The extraction temperature was chosen based on the standard Czech methodology for soil drying (ISO 11 465, 1998), which is consistent with standard methodologies used in the UK (BSI 1377: 105 ± 5 °C) and US (ASTM D2216: 110 ± 5 °C). Values exceeding 100 °C have to be chosen as pore water remains in the soil when temperatures below 100 °C are used

(O’Kelly 2004, 2005). The water vapour is then condensed by tap water at a temperature of 8 °C. Usage of tap water for cooling is motivated by the following reasons

- a) its availability;
- b) temperature of cooling water is close to the ambient air dew temperature (preventing an appearance of ambient air condensation on the cooling loops and hence, possible sample contamination);
- c) prevention from frost formation inside the apparatus, which otherwise increases the risk of blocking the inlet pipes, damaging the glass parts, and causing the difficulty of extracted sample handling (prior to the sample handling, frost on the cooler and collecting vessel walls has to be melted);
- d) with respect to the vapour pressure at the extraction temperature (105 °C: 121 kPa), there is no apparent difference in the extraction rates or residual soil moisture at the equilibrium with the cooling circuit operated at 8 °C (1 kPa) or -10 °C (0.3 kPa).


110 2.2 Description of the apparatus

The newly designed apparatus (Fig. 1a) is composed of three main system units – heating, cooling and air circulation (Fig. 2). The apparatus has four separate circuits for simultaneous water extraction from four different soil samples.


The heating system comprises a standard kitchen oven (model VT 332 CX; MORA MORAVIA s. r. o., Czechia) housing four evaporation chambers – stainless steel boxes equipped with airtight insulation. Each box has two openings, one for a dry air inlet and the other for a moist air outlet. The soil sample inside the box is placed on a stainless-steel wire-mesh bed providing good contact between the sample and air, which enhances the water evaporation rate (Fig. 1b). The dry air is led to the evaporation chamber through a silicone rubber tube coiled inside the oven; its length (~ 2 m) is sufficient to preheat the air close to the oven temperature (Fig. 1c). The hot and moist air from the evaporation chamber is led through the insulated silicone tube to the cooling system; the length of the outlet tubes is as short as possible to minimize the heat losses and prevent undesired water condensation. To monitor the extraction process, a temperature sensor is installed inside each box close to the air outlet.

The cooling system consists of three glass components – spiral cooler, custom-made connecting part and jacketed collecting vessel (Fig. 3). Two separate cooling water circuits are used for the spiral coolers and for the collecting vessels (Fig. 2).

The cooled and dried air from the cooling system is fed back to the evaporation chamber by means of the air circulation system comprising two regulated high-speed fans per circuit ensuring the air flow rate of ~ 10 L/min. The temperature sensors and fan speed in each circuit are monitored by the control unit running on the Arduino platform. The apparatus is complemented by an air diaphragm pump that can be connected to any circuit to flush the circuit with fresh dry air to remove possible residual moisture in the apparatus prior to extraction and thus achieve more accurate results. The tests presented in this work were carried out without the use of this pump. However, for the extraction of soil water with significantly different isotopic compositions, the execution of an initial purge between extractions would be appropriate.

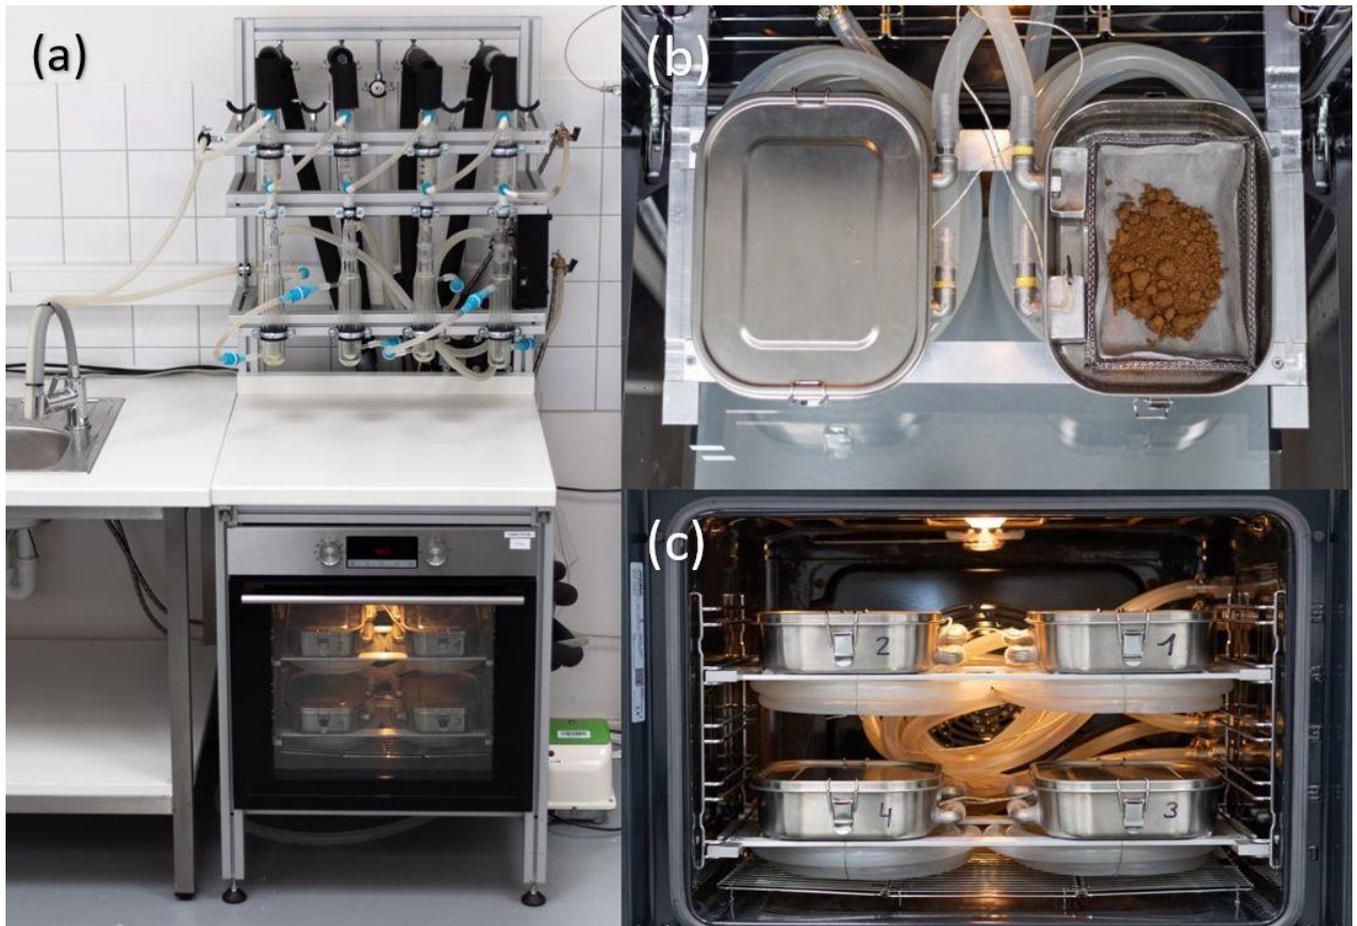

135 **Figure 1: a) Photo of the proposed CASWE apparatus; b) detail of the heating chamber with wire-mesh bed and aluminium fabric bedding; c) internal arrangement of heating chambers and coiled supply hoses.**

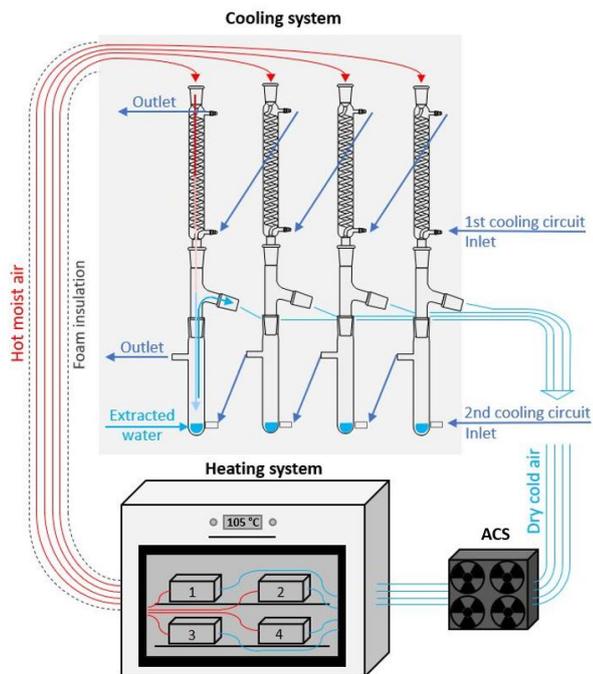

140 **Figure 2:** A simplified diagram of three main components of the CASWE apparatus (heating, cooling and air circulation systems (ACS)). The apparatus consists of four separate drying circuits and two cooling circuits.

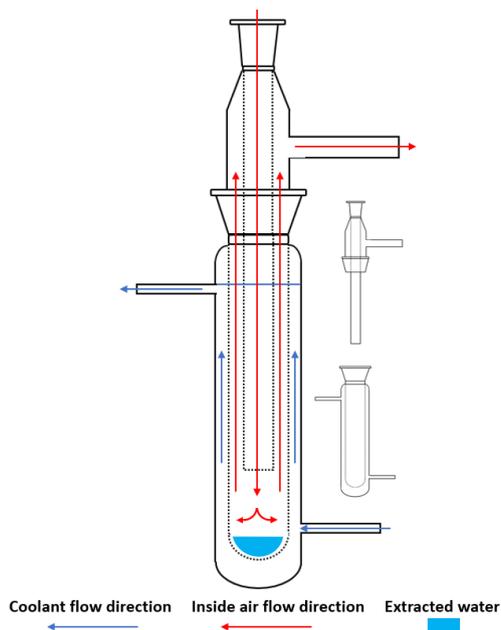


Figure 3: Lower part of the cooling system – custom-made connecting part and jacketed collecting vessel. The arrows indicate the flow direction within the assembly. Thumbnails show individual parts before assembly.

145 **2.3 Extraction procedure**

Soil samples are inserted on the wire bed of the evaporation chambers. A target temperature of 105 °C is reached approximately within 15 minutes. This initiates the first intensive part of the drying process, during which both cooling circuits operate and most of the water is extracted. The upper cooling circuit (Fig.2) is disconnected once the spiral cooler starts to dry out. The extraction continues with the bottom cooling circuit only. During this time, residual moisture in the apparatus is collected in
150 the cooled collection vessel.

The extraction is complete when there are no visible signs of condensation elsewhere than in the collection vessel. To check the completeness of the extraction, the recovery ratio was calculated for each extraction, by comparing the weights of added and extracted waters. For complete checking of the functionality of the apparatus, some soil samples were weighed after pre-oven-drying and after extraction. Depending on the sample type, water content, and size, the extraction time intervals
155 ranged from 3 to 6 hours per sample. Between each extraction, the circuit is disassembled to retrieve the extracted water from the collection vessel and exchange soil samples. Thorough mixing of the sample before pouring from the collection vessel and catching all droplets from the walls to ensure the homogeneity of the sample is needed. The collection vessel must then be dried to avoid contamination during further extraction.

2.4 Functional tests

160 In total, six functional tests were performed. All the tests aimed at recovering the same amount of water that was used with no changes in its isotopic composition. The first test served for a verification of the principle of extraction and for checking waterproofing and airtightness of the apparatus. The remaining five tests verified the accuracy of the extraction with soil samples via spike experiments. In these experiments, disturbed soil samples were pre-oven-dried (105 °C for 24 h), spiked in the evaporation chamber with a specific amount of labelled water, mixed and then left to equilibrate for two hours. Five sets
165 of spike experiments with different soil textures were performed as soil texture plays a crucial role during soil water extraction (Orlowski et al., 2016a). In each spike experiment, identical samples were rewetted repeatedly (with the exception of artificially prepared sandy clay, described below) to reveal any shift in the isotopic composition of the extracted water and thus to eliminate any possible influence of the residual water from the sample due to incomplete drying prior to extraction. This follows a procedure described in Gaj et al. (2017).

170 Six consequent tests (Tab. 1) were carried out in the following way:

First test: Water of known isotopic composition and quantity (15 mL) was poured into the heating chambers.

Second test: Disturbed soil samples (65 g each) of loamy sand texture were spiked with 15 mL of water of known isotopic composition. The soil samples were reused and re-hydrated 3 times.

Third test: The procedure was the same, as in the second test, using sandy loam soil samples.

175 Fourth test: 40 g samples were prepared in the laboratory by mixing sand (60 %) with clay (40 %) and spiking with 10 mL of known isotopic composition. A lower sample size and water amount were used to reduce the corresponding extraction

time. In this case, a new sample was prepared for each extraction run due to concerns of possible sealing of the sample after extraction, which would make it difficult to re-hydrate.

180 Fifth and sixth tests were used to verify the functionality of the method with a lower water content (10 %). To the fifth test, disturbed soil samples (150 g each) of silt loam texture were spiked with 15 mL of water of known isotopic composition. Since we did not observe any significant sealing in the previous test the soil samples were reused and re-hydrated 2 times. The same procedure was used for the sixth test, only with a different soil texture (clay) where the samples were reused and re-hydrated 3 times.

185 **Table 1: Sample properties to verify the apparatus functionality.**

Test	Sample (g)	Water (mL)	Soil (g)	W (%)	θ (%)	Soil texture	% sand	% silt	% clay
1st	15	15	-	-	-	-	-	-	-
2nd	80	15	65	23	18.75	Loamy sand	85.5	5.5	9
3rd	80	15	65	23	18.75	Sandy loam	56.5	34.8	8.7
4th	50	10	40	25	20	Sandy clay	60	-	40
5th	165	15	150	10	9	Silt loam	16	60	24
6th	165	15	150	10	9	Clay	28	28	44

W is gravimetric water content and θ is volumetric water content.

For each test there was used labelled water slightly differing in stable isotope composition (Tab. 2), which was analysed at the Institute of Hydrodynamics (Czech Academy of Sciences) with the L2140-i isotope analyser (Picarro Inc., US). Standard mode (precision of ± 0.03 ‰ and ± 0.15 ‰ for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively) was used with 6 injections per sample with the first 3 injections discarded. The isotope ratios are reported in per mil (‰) relative to Vienna Standard Mean Ocean Water (VSMOW) ($\delta^2\text{H}$ or $\delta^{18}\text{O} = (R_{\text{sample}}/R_{\text{standard}} - 1) \times 1000$ ‰, where R_{sample} is the isotope ratio of the sample and R_{standard} is the known reference value (i.e., VSMOW) (Craig, 1961)). The target accuracy of the method is given by the limit of ± 0.2 ‰ for $\delta^{18}\text{O}$ and ± 2 ‰ for $\delta^2\text{H}$, which is considered reasonable for hydrologic studies (Wassenaar et al., 2012; Orłowski et al., 2016b). The terms ‘shift’ and ‘bias’ were used for an evaluation of the results, where ‘shift’ means a difference from the labelled water and ‘bias’ indicates the standard deviation of the data. Please note that these terms are often replaced by the terms accuracy (shift) and precision (bias) in some studies (Revesz and Woods, 1990; Koeniger et al., 2011; Ignatev et al., 2013; Zhue et al., 2014; Sprenger et al., 2015; Gaj et al., 2017).

3 Results

200 3.1 Waterproof and airtightness test

To test the extraction method and the water- and air-tightness of the apparatus (1st test), 15 mL of water of known isotopic composition was used. Extraction of this water amount took on average 5 hours. The resulting recovery ratio after the extraction process averaged 99.7 % of the volume of the used labelled water. The remaining water fractions were given by the sum of the residual thin layer of moisture left on the walls inside the collection vessel during the transfer of the samples into the vials, residual moisture inside the apparatus and possible diffusion through the silicon tubing. The stable isotope composition of labelled water used for this test was -9.61 ± 0.01 ‰ for $\delta^{18}\text{O}$ and -66.34 ± 0.05 ‰ for $\delta^2\text{H}$ (N=4) (Tab. 2, Fig. 4). The total average of the mean stable isotope composition of extracted water (N=13) was shifted by -0.04 ‰ (bias ± 0.06 ‰) and 0.06 ‰ (bias ± 0.35 ‰) for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively.

3.2 Spike experiments

210 The other five tests – spike experiments – verifying the functionality of the extraction took on average 3 hours for the loamy sand, 4 hours for the sandy loam, 5 hours for the sandy clay and silt loam, and 6 hours for the clay samples. The resulting recovery rate after the extraction process attained on average 99.3 % of the used labelled water volume (Tab. 2). The remaining water fractions were given, analogously as before, by the sum of the residual thin layer of moisture left on the walls inside the collection vessel during the transfer of the samples into the vials, residual moisture inside the apparatus and possible diffusion through the silicon tubing. The sixth test represented the only exception (clay soil from the Halaba area, Central Ethiopia), where the recovery rate often exceeded 100 %. Since a similar phenomenon was not observed with the other samples and the apparatus was tested for possible leakage (which was not found), we hypothesize that this error is due to the extreme chemical composition of the selected samples (potential release of crystalline water from the soil itself) or insufficient pre-oven-drying (despite applied 72 hours).

220 In the second test (loamy sand), the stable isotope composition of labelled water was -9.22 ± 0.01 ‰ for $\delta^{18}\text{O}$ and -64.56 ± 0.04 ‰ for $\delta^2\text{H}$ (N=3). The average obtained isotopic composition was depleted by 0.03 ± 0.08 ‰ in $\delta^{18}\text{O}$ and enriched by 0.4 ± 0.34 ‰ in $\delta^2\text{H}$ (N=11) (Tab. 2, Fig. 4). As in the first test, the $\delta^{18}\text{O}$ values were slightly depleted but almost matched the labelled water. However, the $\delta^2\text{H}$ values were relatively enriched (Fig. 4; Tab. A2).

In the third test (sandy loam), the stable isotope composition of labelled water was -9.37 ± 0.01 ‰ for $\delta^{18}\text{O}$ and -64.70 ± 0.05 ‰ for $\delta^2\text{H}$ (N=3). The mean isotope composition of extracted water was enriched for both isotopes but with no statistical significance for $\delta^{18}\text{O}$ (Tab. A2). The average shift and bias attained 0.03 ± 0.13 ‰ for $\delta^{18}\text{O}$ and 0.51 ± 0.5 ‰ for $\delta^2\text{H}$ (N=15). Compared to the second test, the variance of the values increased.

In the fourth test (sandy clay), the stable isotope composition of labelled water was -9.54 ± 0.01 ‰ for $\delta^{18}\text{O}$ and -75.92 ± 0.05 ‰ for $\delta^2\text{H}$ (N=3). The mean isotope composition of extracted water was enriched for both isotopes but with no statistical significance for $\delta^{18}\text{O}$. The values of $\delta^{18}\text{O}$ increased by 0.03 ± 0.11 ‰ and of $\delta^2\text{H}$ by 0.68 ± 0.58 ‰ (N=11).

In the fifth test (silt loam), the stable isotope composition of labelled water attained -9.35 ± 0.02 ‰ for $\delta^{18}\text{O}$ and -66.06 ± 0.05 ‰ for $\delta^2\text{H}$ (N=3). The mean isotope composition of extracted water was enriched for both isotopes but with no statistical significance for $\delta^{18}\text{O}$. The values of $\delta^{18}\text{O}$ increased by 0.07 ± 0.11 ‰ and of $\delta^2\text{H}$ by 1.31 ± 0.55 ‰ (N=8).

235 In the sixth test (clay), the same labelled water was used as in the fifth test. The mean isotope composition of extracted water was enriched for both isotopes but with no statistical significance for $\delta^{18}\text{O}$. The values were shifted by 0.01 ± 0.25 ‰ for $\delta^{18}\text{O}$ and 0.96 ± 0.39 ‰ for $\delta^2\text{H}$ (N=12).

The Kolmogorov-Smirnov test at 5% significance level was performed for all sets of the results to determine the normality of the data. The measured data for all six tests exhibited a normal distribution. Furthermore, one sample t-test was performed at 5% significance level to determine whether the extracted values were significantly different from the standard used in the given test. For the first set of the results (extraction test with water only), the average of the data is not statistically different from the standard used. In the remaining extraction tests, using soil, the mean is always statistically identical to the standard used only in the case of $\delta^{18}\text{O}$. In the case of $\delta^2\text{H}$ values, the null hypothesis was always rejected. Furthermore, the data variance of $\delta^2\text{H}$ is increasing with a higher amount of fine particles in the soil (silt, clay). The statistical test results are summarized in Table A2.

245 Since the normality test, which is a prerequisite for the t-test, may not be valid on such small data sets, we also performed the Bootstrap analysis which does not require this assumption. This analysis calculates the 95% confidence interval in which the true value is located (Fig. A3). The results of this analysis were consistent with the results of the t-test.

Table 2: Summary of the individual test results.

Test	Type	N	$\delta^{18}\text{O}$ (‰)	SD (‰)	$\delta^2\text{H}$ (‰)	SD (‰)	Sample type	Extraction time (h)	Recovery rate (%)
1st	L	4	-9.61	± 0.01	-66.34	± 0.05	Water	5	99.7
	E	13	-9.65	± 0.06	-66.28	± 0.35			
2nd	L	3	-9.22	± 0.01	-64.56	± 0.04	Loamy sand	3	99.5
	E	11	-9.25	± 0.08	-64.16	± 0.34			
3rd	L	3	-9.37	± 0.01	-64.70	± 0.05	Sandy loam	4	99.2
	E	15	-9.34	± 0.13	-64.19	± 0.50			
4th	L	3	-9.54	± 0.01	-75.92	± 0.05	Sandy clay	5	99.3
	E	11	-9.51	± 0.11	-75.24	± 0.58			
5th	L	3	-9.35	± 0.02	-66.06	± 0.05	Silt loam	6	99.1
	E	8	-9.27	± 0.11	-64.75	± 0.55			
6th	L	3	-9.35	± 0.02	-66.06	± 0.05	Clay	6	99.9
	E	12	-9.34	± 0.25	-65.11	± 0.39			

L and E indicate the labelled and extracted water used in the test, respectively. N stands for the number of samples.

The isotope ratios ($\delta^{18}\text{O}$, $\delta^2\text{H}$) and their standard deviations (SD) are reported in per mil (‰) relative to Vienna Standard Mean Ocean Water (VSMOW). The extraction times quoted are average times valid for the disturbed soil samples and may vary with other samples depending on the sample size, texture and water content. The recovery ratio was calculated as the weight of extracted water divided by the weight of the added labelled water and multiplied by 100.

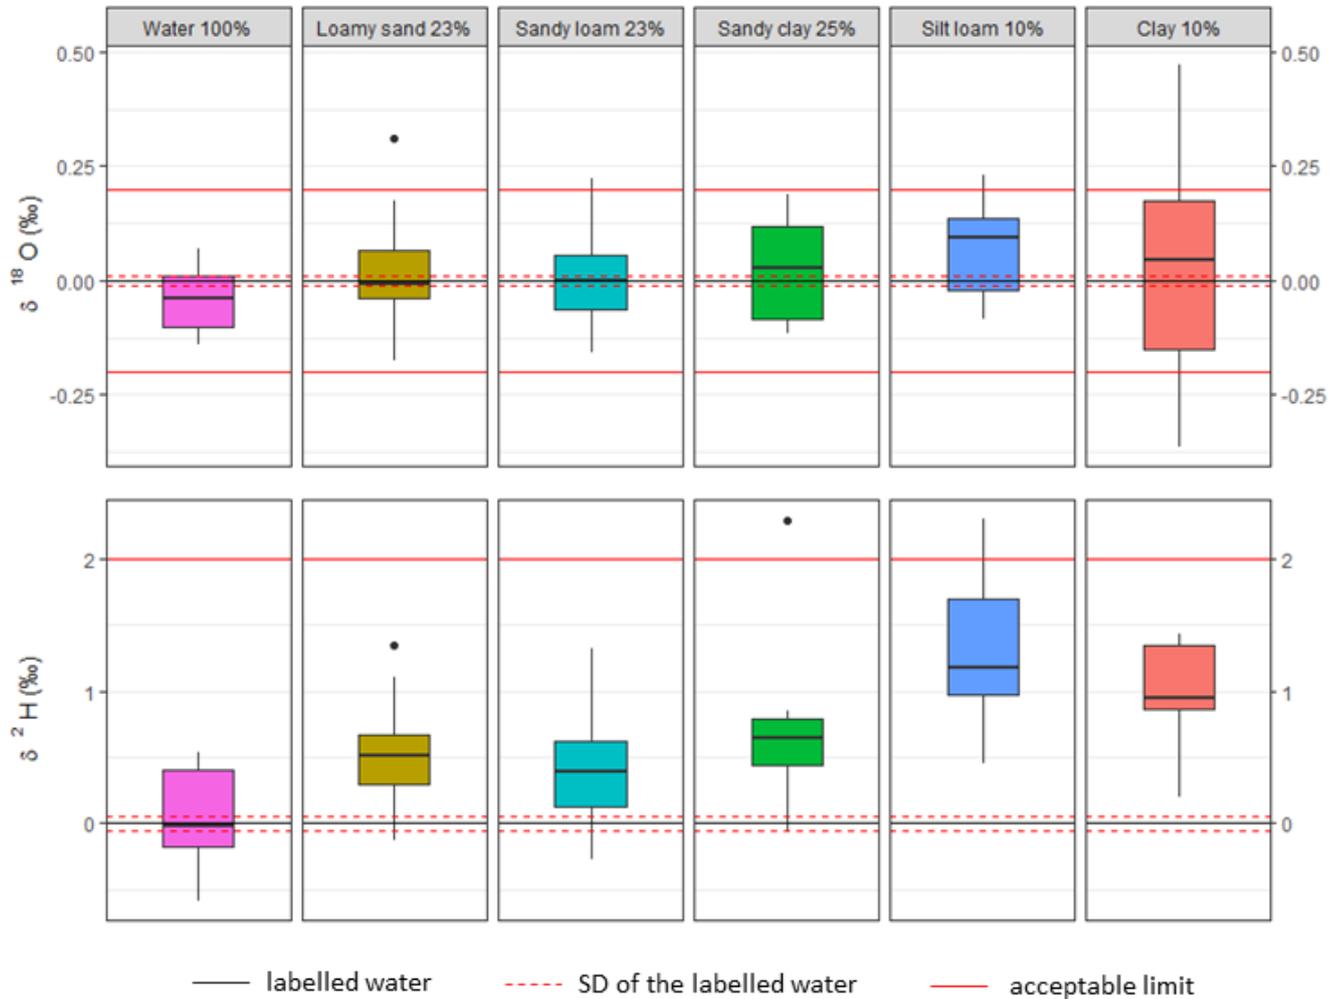


Figure 4: Relative deviation of the isotopic ratio of extracted water compared to the labelled water and its standard deviation. For better clarity, all results are recalculated as if the used labelled water had a VSMOW composition. The acceptable limits are represented by the error of ± 0.2 ‰ for $\delta^{18}\text{O}$ and ± 2 ‰ for $\delta^2\text{H}$, which is considered reasonable for hydrologic studies (Wassenaar et al., 2012; Orłowski et al., 2016b).

4 Discussion

4.1 Residual moisture in the apparatus

265 The apparatus is designed to handle an entire standard soil core (100 cm³). The sample size is limited only by the volume of the heating chamber (roughly 400 cm³ of usable space) and the size of the collection vessel (~ 25 mL). An advantage of extracting a bigger soil sample over the smaller ones (e.g. < 10 g) is a much better representation of the sample properties. ~~However, because of this the extraction time and total throughput are lower compared to other methods (e.g. CVE, DVE-LS).~~

270 The larger amount of obtained extracted water with the proposed extraction apparatus lower a potential inaccuracy accompanied by lower sampling amounts in other extraction methods. Additionally, it offers the advantage to run the same extracted water sample using both the Isotope Ratio Mass Spectrometry (IRMS) and the Isotope Ratio Infrared Spectroscopy (IRIS) machines. However, not all water ends up in the collection vessel. Based on the estimated gas volume of 4 L, the ideal gas law and equilibrium conditions at 8 °C, the amount of water left in the circuit is approximately 50 mg. Furthermore, humidity gains and losses can occur during the extraction procedure because of the silicon hoses' permeability. The estimates of humidity losses for the extraction time not exceeding 24 h are less than 0.5 % of the total sample mass, regardless of the extracted water amount. The estimates are based on the water-silicone solubility and permeability (Barrie and Machin, 1969),

275 supposing 50 % relative humidity in the room outside the extractor, and 8 °C cooling water. Under these conditions the absolute air humidity inside the extractor is higher (during the proceeding extraction) or equal to the ambient air humidity, allowing for minor sample losses (< 0.5 %) via vapour permeation when the extraction proceeds, and no losses once the sample is almost or completely dry. The hoses can also absorb water vapour from the air. The water absorbed in the silicone hoses is released back into the circuit when heated (by calculation estimated to approximately 50 µg). Although silicone hoses may not seem

280 ideal for this purpose, the choice of construction materials was a compromise between handling and operating the extractor and material resistance/neutrality with respect to the extracted water. Despite the potential sample gains/losses, these amounts are still marginal compared to the amount of extracted water, so it does not exhibit a major effect on the results (as demonstrated).

285 Most of these error sources can be suppressed by using larger sample sizes. For even more accurate results, it might help to choose a different construction material (PTFE, stainless steel), to seal entirely the apparatus during idle time, pre-drying the empty apparatus or purging the apparatus with dry air, or nitrogen (as inert gas). However, the extraction procedure would be more complicated and the nuances that this would resolve are negligible in comparison to other factors (e.g. the amount of clay in the sample, the accuracy of measurements of the stable isotope composition itself) which will affect the final composition more significantly.

290 Thorough mixing of the sample before pouring from the collection vessel and catching all droplets from the walls to ensure the homogeneity of the sample is necessary. Because of that, the water adheres to the walls of the collecting vessel, whereby the residual amount always remains there while pouring the sample into the vials. This adhered water contributes significantly to the incomplete recovery rate and often covers the majority of this error. Since the sample was mixed

(homogenized) during the collection of all residual droplets on the walls of the collection vessel, we assume that the residual
295 film in the glass will not affect the isotopic composition of the sample but only the recovery ratio.

With respect to the Rayleigh distillation principle (Dansgaard, 1964; Araguás-Araguás et al., 1995), the observed
shift of extracted soil water towards enriched values of the heavier isotopes also points to imperfect collection of extracted
water. The slight enrichment indicates incomplete water condensation and the presence of lighter isotopes (as quantified above)
inside the apparatus as also evidenced by the high but incomplete recovery rate. Complete evaporation of the soil water is
300 confirmed by comparison of soil sample weights (weight after extraction for selected samples was equal or slightly lower to
the sample weight after pre-oven-drying).

As discussed earlier, two following factors can notably influence the composition of the collected water, thus the
reliability of the proposed method: insufficient tightness of the whole circuit (joints, etc.) and permeability of the pipes made
of silicon. The absence of the former factor is checked by the recovery rate close to 100 %. The latter factor – possible sample
305 contamination with ambient moisture comprising substantially lighter isotopic composition (~ -13 ‰ and -125 ‰ for $\delta^{18}\text{O}$ and
 $\delta^2\text{H}$, respectively) – is almost completely suppressed, as the experimental results exhibit only negligible change in the labelled
water isotopic composition. Moreover, the observed shift in the water composition (enrichment by heavier isotopes) indicates
marginal sample fractionation instead of its contamination by ambient moisture.

4.2 Extraction time

310 For many methods, extraction time often plays a significant role in the resulting isotopic composition of the sample (Revesz
and Woods, 1990; West et al., 2006; Zhu et al., 2014; Hendry et al., 2015; Orłowski et al., 2018; Orłowski and Bauer, 2020).
In this case, no significant differences were observed between ending the extraction at the time when the circuit is visibly dry
and prolonging the extraction by an hour or more, because the same dry, cold air is still flowing when the extraction is
completed. Once the extraction is complete, the apparatus reaches an equilibrium state at which the amount and composition
315 of the water sample are fixed. The proposed method is one of the slower ones compared to other extraction methods. The
extraction time using the CVE method varies from 15 minutes (Orłowski et al., 2018) to 6 hours (Mora and Jähren, 2003).
However, it should be added that for the CVE method, sample sizes of 10-20 g are used and only a few mL of water are
extracted (Tab. 3), whereas in the presented method extraction of the sample size attained up to 150 g and extracted liquid
water amounts up to 15 mL. The extraction time is therefore longer and varies between 3 to 6 hours depending on the soil
320 texture (the larger porosity of the sample reduces the extraction time significantly), water content and sample size. The presence
of pores in the soil and thus larger surface area for evaporation is also the reason, why the extraction time of some soil samples
was shorter than the extraction of water alone (1st test). The soils are dried on a manufactured bed to allow air to reach the
soil sample from all sides. Contrarily, the water sample was placed in a small stainless steel bowl enabling air-water interaction
only on the surface (upper side). By making this surface larger for the soil, the extraction is faster. Also, the soil itself exhibits
325 a higher thermal conductivity than air.

In the case of low soil moisture, a larger soil sample should be used (to extract at least 7-10 mL of water) resulting in a longer extraction time. The extraction times quoted above are average times valid for the samples used in this study and may vary with other samples (especially undisturbed samples, or samples with different water content).

330 In large-scale studies, higher sample throughput is an important factor. For these purposes, apparatuses with higher throughput that can handle 30 or more samples in an 8-hour working day are used (Goebel and Lascano, 2012; Orłowski et al., 2013; Yang et al, 2023). The proposed apparatus has currently only four circuits, hence four soil samples can be processed simultaneously. Depending on the soil type and water content a maximum of two runs per day can be processed. ~~The apparatus is suitable for smaller high precision studies where unambiguous determination of the water origin is required.~~ Reduction of the sample size could increase the throughput resulting in a reduction of the extraction time, but it could be projected in higher
335 inaccuracy of the results. ~~To apply this method in large scale studies, it would be necessary to use more apparatuses, change the heating source and use a larger oven to accommodate more heating chambers or increase the air circulation speed in the apparatus.~~

4.3 Comparison of soil water extraction approaches

In order to compare the proposed method of soil water extraction with other approaches, we gathered the results presented in
340 other references. The results proved (Tab. 3 and Fig. 5) that the presented method is able to fit safely within an acceptable range of accuracy (± 0.2 ‰ for $\delta^{18}\text{O}$ and ± 2 for $\delta^2\text{H}$ ‰ (Wassenaar et al., 2012)) which is for other methods rather problematic, even if different soil types are used. For example, with a clay-rich soil sample, the DVE-LS method (Wassenaar et al., 2008) achieves low standard deviations (± 0.02 ‰ and ± 0.5 ‰ for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively) but the shift in the data is at (+ 2 ‰ for $\delta^2\text{H}$) or beyond (+ 1 ‰ for $\delta^{18}\text{O}$) the limit of acceptability. McConville et al. (1999) obtained very accurate results with the
345 direct equilibrium method (0.1 ± 0.12 ‰ for $\delta^{18}\text{O}$), but only a sandy soil was studied. A comparison with the most commonly used method, CVE, is difficult, due to the huge dispersion of values presented by different laboratories (Orłowski et al., 2016b, 2018). In this study, we used the reported values of Yang et al. (2023), Newberry et al. (2017) and Koeniger et al. (2011) as a reference. The reported shifts in the data were between -0.16 to -0.59 ‰ and -2.6 to 2 ‰ for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively and the deviation was in the range of ± 0.14 to 0.4 ‰ and ± 1.3 to 3 ‰ for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively, where the most problematic
350 samples exhibited high content of clay particles. Based on our tests carried out so far, it seems that in some cases the obtained shifts are up to one order of magnitude lower than the shifts in the above studies. The reported values are depleted in both isotopes which contradicts the values reported in this study (where especially the $\delta^2\text{H}$ values are rather enriched). Orłowski et al. (2016b) showed, that in the case of extraction from sandy samples, the extracted water by the CVE method is almost identical to the applied label water. However, as the proportion of clay particles in the sample increases, the accuracy
355 significantly decreases and the difference with the labelled water for clay samples is more than 1.5 ‰ and 12 ‰ for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively. In this study, with an increasing amount of clay in the sample only a gradual shift in isotopic composition is visible. For both isotopes, there is a higher enrichment of heavy isotopes in the sample and the dispersion of the values increases. Only the $\delta^2\text{H}$ is statistically different from the labelled water used (Tab. A2, Fig. A3).

Many laboratories have considerable problems with the extraction of water itself (Orlowski et al., 2018). The best-
 360 reported results of extracted water in the interlaboratory study by Orlowski et al. (2018) were 0.1 ± 0.1 ‰ for $\delta^{18}\text{O}$ and $-0.8 \pm$
 0.4 ‰ for $\delta^2\text{H}$, which was again almost an order of magnitude different from the results presented in this study. Only 2 of 16
 laboratories in the CVE interlaboratory comparison study presented comparable results. This indicates that the problem with
 accuracy is not caused by the method itself (CVE can give very accurate results), but it is connected with the possibility of
 how to arrange the settings of the apparatus. Minor differences may occur due to the measurement of the isotopic composition
 365 itself, depending on the instrument and method used (Penna et al., 2010, 2012).

The method providing comparable results with this study is a modification of the CVE method presented by Ignatev
 et al. (2013), using He as carrier gas instead of water vapour diffusion only. In both cases, mass transfer coupled with gas flow
 (air in the presented study and He in Ignatev's case) was shown to be more efficient compared to diffusive mass transfer
 (Ishimaru et al., 1992) and hence, more accurate results can be achieved. The reported values by Ignatev et al. (2013) are 0.03
 370 ± 0.08 ‰ and 0.7 ± 0.7 ‰ for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively. In comparison with the proposed method, there is a higher shift for
 $\delta^{18}\text{O}$ values but a lower shift in $\delta^2\text{H}$ values in the He-purging method. However, it should be noted that these differences of
 hundredths ($\delta^{18}\text{O}$) to units of tenths ($\delta^2\text{H}$) are mostly within the measurement inaccuracy of an isotope analyser.

Another step, in our opinion, possibly affecting the CVE results (that is not present in the proposed procedure) is the
 actual vacuum formation in the CVE apparatus. Although in the prevailing majority, the soil sample is inserted into the
 375 apparatus frozen, there is no guarantee that evaporation or sublimation does not occur at very low pressures.

Table 3: Comparison of the reported results of selected soil water extraction methods in different studies.

Method	Study	Sample type	Average $\delta^{18}\text{O}$ shift \pm SD (‰)	Average $\delta^2\text{H}$ shift \pm SD (‰)	N	T (min)	Spiked water (mL)
Extraction with accelerated solvent	Zhu et al. (2014)	unknown soil	0.36 ± 0.37	3.6 ± 0.89	1*	30	1
Azeotropic distillation	Revesz & Woods (1990)	Sandy soil	$0.35\text{--}0.77 \pm 0.2$	$2\text{--}3.2 \pm 2$	1*	25	3
Ultrasonic centrifugation	Zhue et al. (2014)	unknown soil	$0.49 \pm -$	$1 \pm -$	10	40	1
Centrifugation	Leaney et al. (1993)	Clayey soil	$0\text{--}3 \pm -$	-	-	-	-
Direct equilibrium	Scrimgeour (1995)	unknown soil	$-1.5\text{--} -0.11 \pm 0.4$	$- \pm 2$	1	16	-
Direct equilibrium	McConville et al. (1999)	Sandy soil	0.1 ± 0.12	-	1	15	-

Direct equilibrium	Wassenaar et al. (2008)	Clay-rich soil	1 ± 0.02	2 ± 0.5	1	5	-
ACVD	Yang et al. (2023)	Clay loam	-0.16 ± 0.14	-2.6 ± 1.3	14	240	1.2
CVE	Koeniger et al. (2011)	Sandy soil	$- \pm 0.4$	$- \pm 3$	12	15	0.5
CVE	Newberry et al. (2017)	Sandy soil	$-0.59 \pm -$	-	6	90	3
CVE	Orlowski et al. (2018)	Water	0.1 ± 0.1	-0.8 ± 0.4	24	90	2
He-purging	Ignatev et al. (2013)	Clay & silt	0.03 ± 0.08	0.7 ± 0.7	12	180	1.5
	1st test	Water	-0.04 ± 0.06	0.06 ± 0.35	4	300	15
	2nd test	Loamy sand	-0.03 ± 0.08	0.40 ± 0.34	4	180	15
CASWE (proposed method)	3rd test	Sandy loam	0.03 ± 0.13	0.51 ± 0.50	4	240	15
	4th test	Sandy clay	0.03 ± 0.11	0.68 ± 0.58	4	300	10
	5th test	Silt loam	0.07 ± 0.11	1.31 ± 0.55	4	360	15
	6th test	Clay	0.01 ± 0.25	0.96 ± 0.39	4	360	15

380 The values represent the average shift from the labelled water used \pm the standard deviation. ACVD stands for automatic cryogenic vacuum distillation, CVE stands for cryogenic vacuum extraction and CASWE stands for Circulating air soil water extraction method. The CVE results from the study by Orlowski et al. (2018) show only the best results achieved in the comparison of CVEs made in that study. Average $\delta^{18}\text{O}$ and $\delta^2\text{H}$ shifts represent the deviation from the mean of used labelled waters. SD stands for standard deviation (bias). T is the extraction time for N samples, that can be processed simultaneously. The number of samples marked with * may vary depending on the size of the apparatus. The last column gives the amount of labelled water used.

385

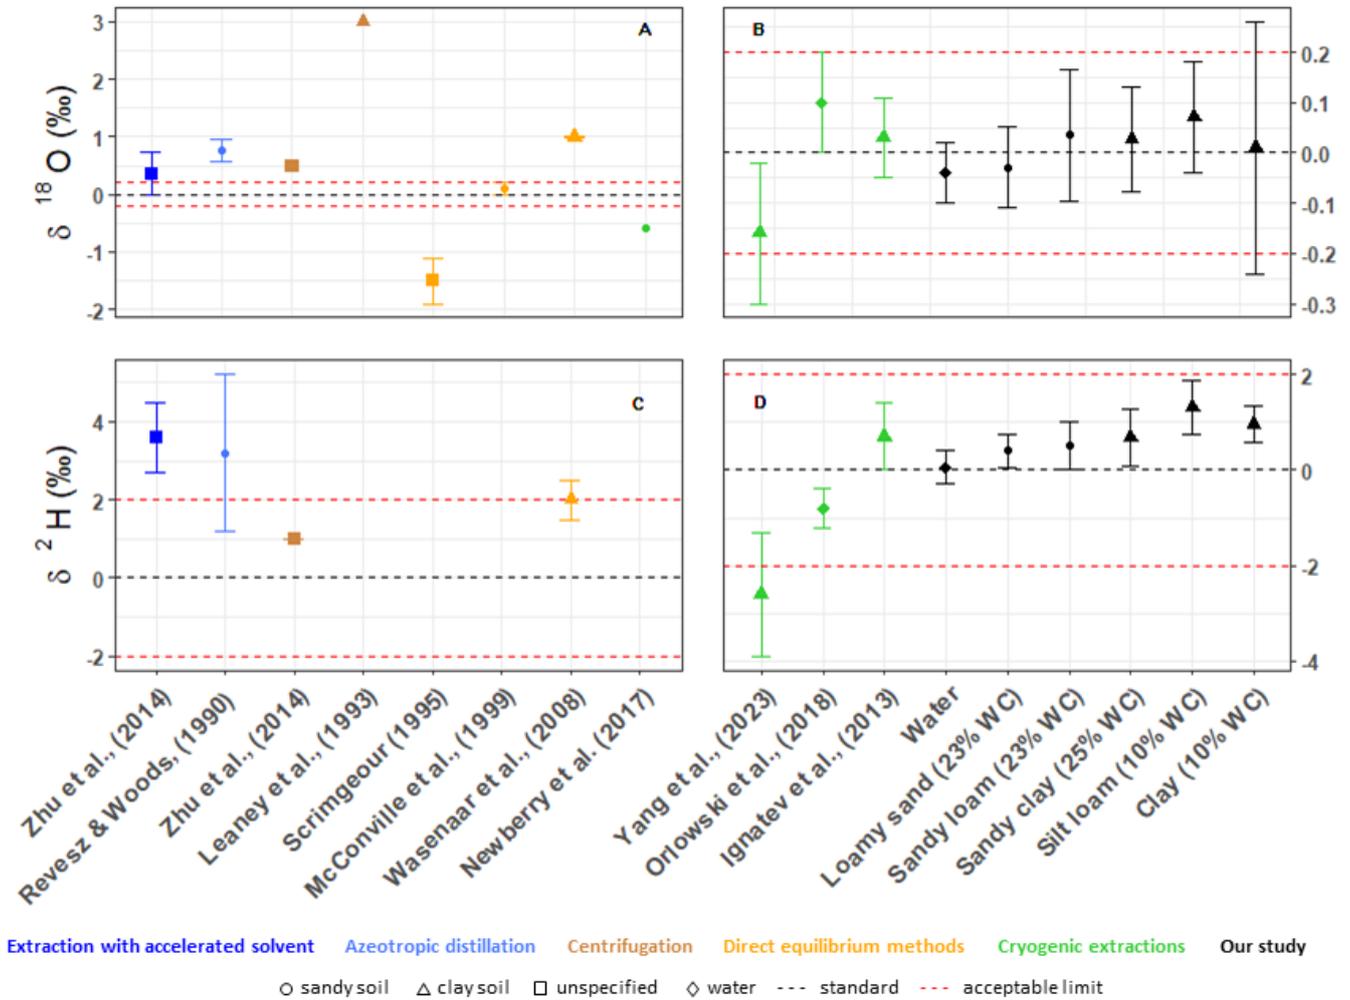


Figure 5: A graphical comparison of the presented results with other methods (A, B for $\delta^{18}\text{O}$; C, D for $\delta^2\text{H}$). Different markings indicate different sample types. The acceptable limits are represented by the error of ± 0.2 ‰ for $\delta^{18}\text{O}$ and ± 2 ‰ for $\delta^2\text{H}$, which is considered reasonable for hydrologic studies (Wasenaar et al., 2012; Orlowski et al., 2016b). The right side of the oxygen graph (B) with more accurate methods has a zoomed y-axis.

4.4 Limitations of the proposed method and future development

The main advantage of the CASWE method consists in the ability to extract water from relatively large (hundreds of grams) soil samples, which reduces the effect of soil heterogeneity and sample handling on the measured isotopic composition. On the other hand, such sample size brings some less favourable effects. In the field, the commonly used narrow soil probes may be insufficient to collect the required amount of soil, which may necessitate the excavation of a larger pit to obtain a sample. This makes the process more complex and time-consuming and extra care must be taken to prevent isotopic fractionation of

the collected samples. Moreover, the larger amount of soil causes a longer extraction time. In this manner, the complications with handling large soil samples restrict the CASWE method utilization.

400

For broader use, it would be necessary to change the apparatus design in order to simultaneously enable parallel treatment of more samples and reduce the extraction time. The latter could be achieved by increasing the air flow circulation rate and reducing the premature condensation inside the pipeline by, for example, improved insulation or additional heating of the tubes. The apparatus could be adapted for medium-scale studies by choosing a different source of heating and inserting additional evaporation chambers.

405

5 Conclusions

410

A new method for soil water extraction – Circulating Air Soil Water Extraction (CASWE) – is presented and the new apparatus developed for this purpose. The method works on the principle of complete evaporation and condensation in a closed circuit. The soil water was successfully extracted from dried and rehydrated soil samples of different textures (loamy sand, sandy loam, sandy clay, silt loam, and clay). Depending on the soil texture, the average shift from the labelled water used ranged between -0.04 and 0.07 ‰ for $\delta^{18}\text{O}$ and 0.4 and 1.3 ‰ for $\delta^2\text{H}$ with the bias ranging from ± 0.08 to 0.25 ‰ and ± 0.34 to 0.58 ‰ for $\delta^{18}\text{O}$ and $\delta^2\text{H}$, respectively. The differences between extracted and used labelled water were often within measurement error of the used isotope analyser. From the test we executed so far, we obtained the results with lower shift than the results reported by other soil water extraction/equilibration methods such as the CVE and DVE-LS methods and up to an order of magnitude lower shift than other methods (extraction with accelerated solvent, centrifugation, azeotropic distillation). This is achieved through the ability to process large soil samples, thereby reducing the effect of soil heterogeneity on isotopic composition of extracted water and suppressing the inaccuracies accompanying the extraction process. However, the developed apparatus has currently a low throughput with a maximum of eight samples a day due to, besides its small capacity, the long extraction times. As a result, its use for fast processing of large sample quantities is limited. It is designed specifically for small-scale high-precision studies where unambiguous determination of the water origin is required. Also, it can be applied as a supplementary method for studies requiring high throughput serving as a reference for calibration of less accurate extraction methods. We believe that further development, leading to an increased throughput, could enable the application of this method also in medium-scale studies and contribute to a deeper understanding of processes in the vadose zone.~~The developed apparatus for this method has a low throughput with a maximum of eight samples a day. The method has proven its versatility in handling various soil types with different soil textures. The results exhibit high accuracy which makes this method suitable for high-precision studies where unambiguous determination of the water origin is required.~~

415

420

425

Appendix

430 Appendix A

This appendix contains two additional tables and one figure. Table A1 shows all measured data from all functional tests. Table A2 presents the statistical results (test of variance, Kolmogorov-Smirnov test and t-test). Figure A3 depicts the results of the Bootstrap analysis.

435 Table A1: Summary of the measured data

Sample No.	1st test (water)				2nd test (loamy sand)				3rd test (sandy loam)	
	Extracted water	Labelled water								
1	$\delta^{18}\text{O}$ -9.74	$\delta^2\text{H}$ -66.10	$\delta^{18}\text{O}$ -9.60	$\delta^2\text{H}$ -66.25	$\delta^{18}\text{O}$ -9.30	$\delta^2\text{H}$ -64.26	$\delta^{18}\text{O}$ -9.23	$\delta^2\text{H}$ -64.62	$\delta^{18}\text{O}$ -9.06	$\delta^2\text{H}$ -63.36
2	-9.68	-66.49	-9.60	-66.38	-9.36	-64.25	-9.22	-64.52	-9.20	-63.74
3	-9.65	-66.93	-9.62	-66.33	-9.26	-64.16	-9.21	-64.54	-9.15	-63.53
4	-9.73	-66.71	-9.61	-66.39	-9.40	-64.68			-9.44	-64.44
5	-9.59	-66.36			-9.22	-64.47			-9.35	-64.08
6	-9.60	-66.52			-9.26	-64.62			-9.47	-64.29
7	-9.71	-66.41			-9.23	-63.89			-9.34	-63.38
8	-9.57	-65.83			-9.15	-63.92			-9.28	-64.31
9	-9.59	-65.92			-9.1	-63.46			-9.43	-64.70
10	-9.54	-65.94			-9.22	-64.04			-9.21	-64.01
11	-9.71	-66.04			-9.25	-64.04			-9.5	-64.97
12	-9.64	-65.81							-9.37	-64.58
13	-9.64	-66.09							-9.53	-64.97
14									-9.31	-64.12
15									-9.41	-64.32
Average	-9.65	-66.28	-9.605	-66.337	-9.25	-64.16	-9.22	-64.56	-9.34	-61.19
Standard deviation	0.06	0.35	0.01	0.05	0.08	0.34	0.01	0.04	0.13	0.5

		4th test (sandy clay)				5th test (silt loam)				6th test (clay)			
Labelled water		Extracted water		Labelled water		Extracted water		Labelled water		Extracted water		Labelled water	
$\delta^{18}\text{O}$	$\delta^2\text{H}$	$\delta^{18}\text{O}$	$\delta^2\text{H}$	$\delta^{18}\text{O}$	$\delta^2\text{H}$	$\delta^{18}\text{O}$	$\delta^2\text{H}$	$\delta^{18}\text{O}$	$\delta^2\text{H}$	$\delta^{18}\text{O}$	$\delta^2\text{H}$	$\delta^{18}\text{O}$	$\delta^2\text{H}$
-9.36	-64.66	-9.64	-75.42	-9.53	-75.85	-9.43	-64.22	-9.34	-66.12	-9.17	-65.28	-9.34	-66.12
-9.37	-64.67	-9.64	-75.98	-9.53	-75.95	-9.25	-63.77	-9.33	-66.02	-9.11	-65.18	-9.33	-66.02
-9.38	-64.77	-9.49	-73.63	-9.53	-75.96	-9.12	-64.41	-9.38	-66.05	-8.88	-65.16	-9.38	-66.05
		-9.65	-75.55			-9.13	-64.78			-9.31	-65.86		
		-9.45	-75.27			-9.24	-64.98			-9.30	-64.64		
		-9.39	-75.28			-9.25	-65.17			-9.70	-65.76		
		-9.62	-75.20			-9.36	-65.06			-9.43	-64.72		
		-9.52	-75.89			-9.41	-65.62			-9.17	-64.65		
		-9.39	-75.31							-9.71	-65.11		
		-9.35	-75.07							-9.37	-65.12		
		-9.51	-75.07							-9.70	-65.09		
										-9.23	-64.70		
-9.37	-64.70	-9.51	-75.24	-9.54	-75.92	-9.27	-64.75	-9.35	-66.06	-9.34	-65.11	-9.35	-66.06
0.01	0.05	0.11	0.58	0.01	0.05	0.11	0.55	0.02	0.05	0.25	0.39	0.02	0.05

Table A2: Statistical test results

Test		Variance	KS p-values	H ₀	t-test p-values	H ₀
1st	$\delta^{18}\text{O}$	0.004	0.870	TRUE	0.052	TRUE
	$\delta^2\text{H}$	0.134	0.837	TRUE	0.553	TRUE
2nd	$\delta^{18}\text{O}$	0.007	0.766	TRUE	0.284	TRUE
	$\delta^2\text{H}$	0.126	0.976	TRUE	0.004	FALSE
3rd	$\delta^{18}\text{O}$	0.018	0.985	TRUE	0.337	TRUE
	$\delta^2\text{H}$	0.270	0.983	TRUE	0.002	FALSE
4th	$\delta^{18}\text{O}$	0.012	0.786	TRUE	0.440	TRUE
	$\delta^2\text{H}$	0.375	0.228	TRUE	0.004	FALSE
5th	$\delta^{18}\text{O}$	0.014	0.933	TRUE	0.121	TRUE
	$\delta^2\text{H}$	0.349	0.978	TRUE	4×10^{-4}	FALSE
6th	$\delta^{18}\text{O}$	0.068	0.850	TRUE	0.909	TRUE
	$\delta^2\text{H}$	0.162	0.761	TRUE	4×10^{-6}	FALSE


440 *KS H₀: The Data set has a normal distribution. T-test H₀: The sample mean is equal to the reference value. TRUE means*
accepting the null hypothesis, and FALSE means rejecting it. The values were rounded to three valid decimal figures
respecting the uncertainty of the experimental errors.


445

450

455

Figure A13: The results of Bootstrap analysis

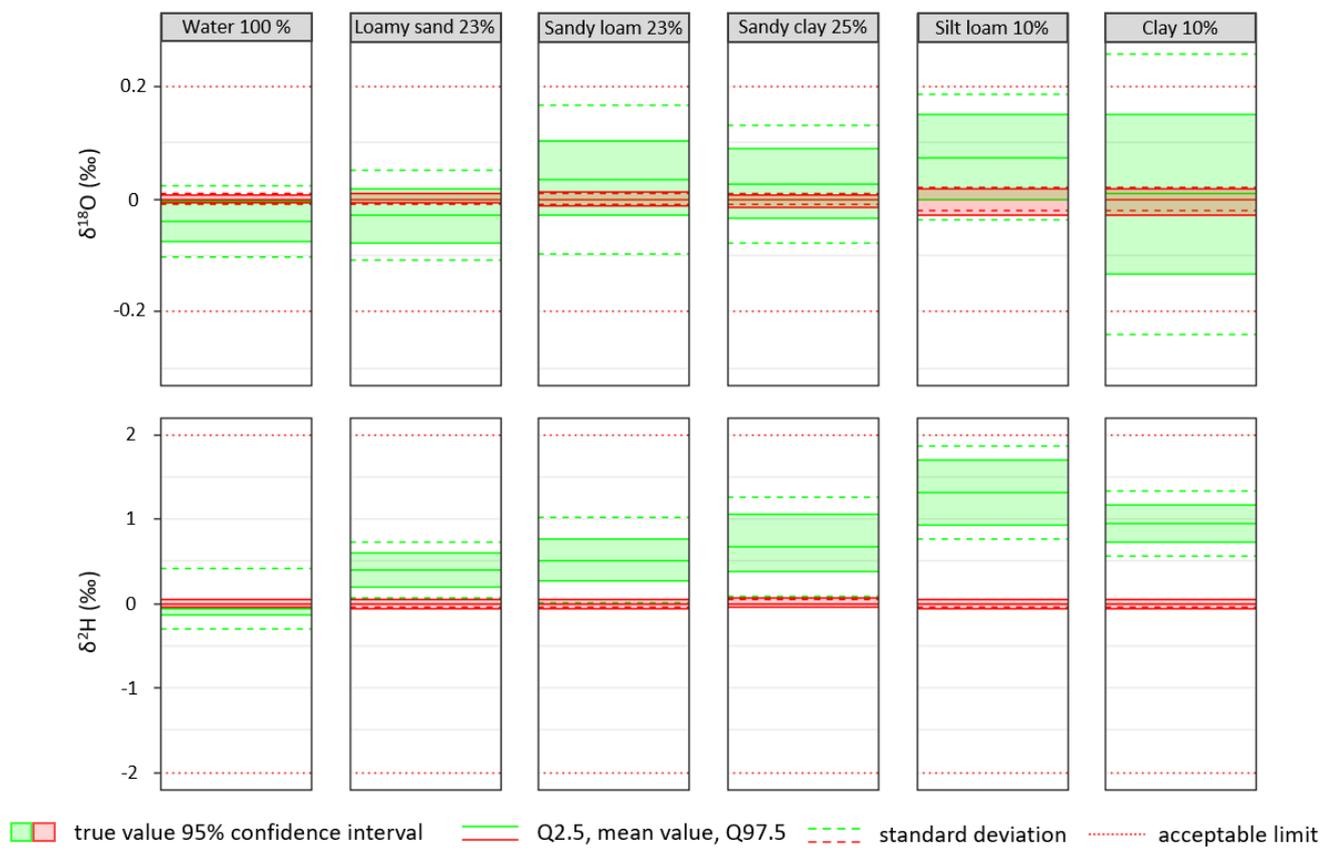

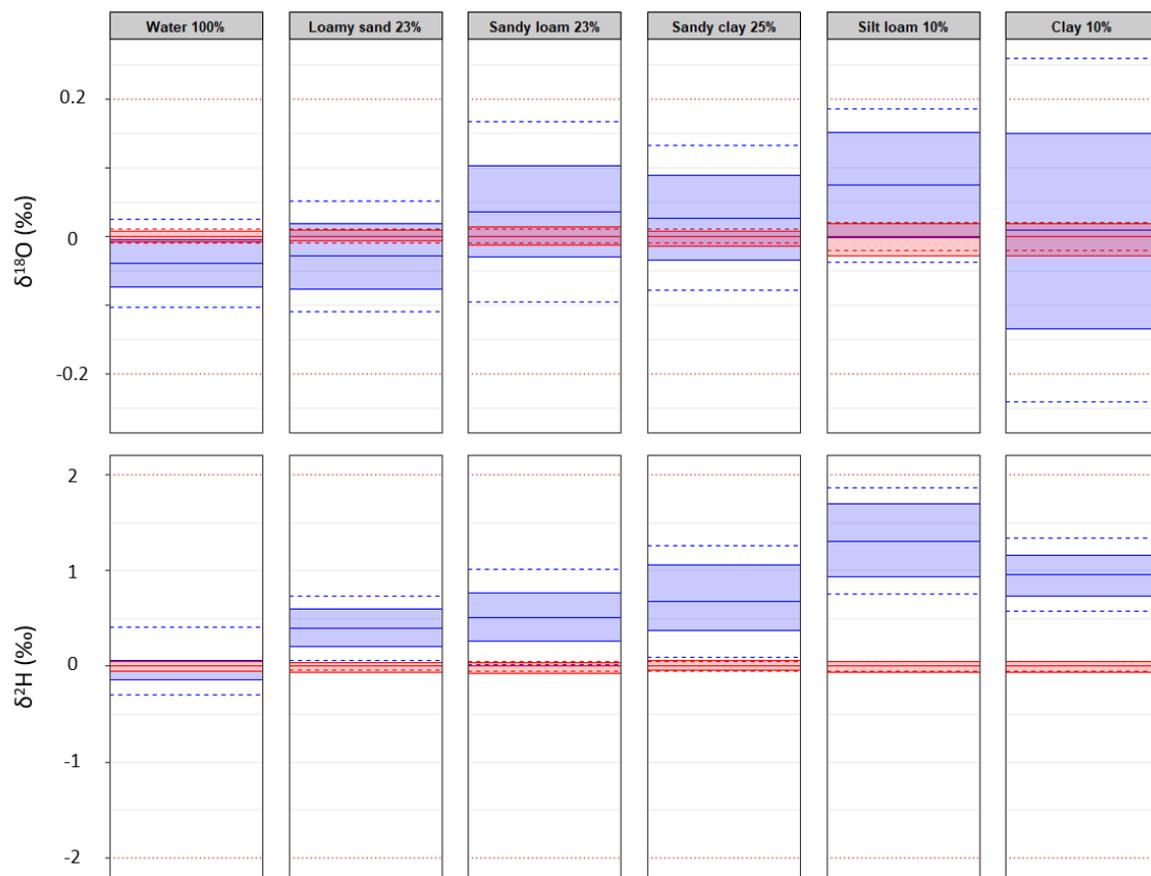

■ true value 95% confidence interval
 — Q2.5, mean value, Q97.5
 - - - standard deviation
 ⋯ acceptable limit

460

BlueGreen colour represents the extracted values and red colour represents the standards used in these tests.

Appendix B

Table B1: List of used components

Component	Type	Supplier	Reference	Quantity	Price [€]
Oven	VT 332 CX	MORA MORAVIA, s.r.o	https://www.alza.cz/mora-vt-332-cx-d6977919.htm?o=1	1	219
Stainless steel bowl	1400 mL	GoEco	https://www.dedra.cz/sk/da30751-dozivotni-celonerezova-doza	4	96
Spiral cooler	Dimroth 14/23	VERKON, s.r.o.	https://www.verkon.cz/chladic-spiralovy-dle-dimrotha/?keyword=dimrotha	4	549

Customized glass	Figure 3	Institute of Chemical Technology in Prague		8	239
Fan	PF40281B1-000U-A99	SUNON	https://www.gme.cz/v/1500620/sunon-pf40281b1-000u-a99-dc-ventilator	8	132
Control unit + accessories	Arduino	Arduino	https://store.arduino.cc/?gad_source=1&gclid=CjwKC A jwkJm0BhBxEiwAwT1AXIKf44cTbvNm3HGYdz Ogppb_OPpGEhaKcywffRo7OP_m2G709MI9RoCE-EQAvD_BwE	-	80
Aluminium profile	40x40 - 104040	ALUTEC KK, s.r.o.	https://katalog.aluteckk.cz/produkt/profil-40x40-104040/	13 m	449
Silicon tube	R973851; R098081	P-LAB	https://www.p-lab.cz/hadicka-silikonova-silnostenna?search=hadice	25 m	510
Glass elbow	14/23	VERKON, s.r.o.	https://www.verkon.cz/koleno-s-nz/?keyword=koleno	4	45
Temperature sensors	(TP-01) K	HOTAIR	https://www.hotair.cz/detail/merici-pristroje/teplomery-a-sondy/termoclanokova-sonda-typu-k-tp-01-s-kevlarovou-izolaci-295cm.html	4	40
Technical stainless steel fabric	2/0.56/1000 mm	Euro Sitex, s. r. o.	https://eshop.eurositex.cz/produkt/281/technicka-tkanina-nerezova-2-0-56-1000-mm/	1	52
	0.05/0.035/1000 mm	Euro Sitex, s. r. o.	https://eshop.eurositex.cz/produkt/257/technicka-tkanina-nerezova-0-05-0-035-1000-mm/	1	73
Hose couplings	R034351	P-LAB	https://www.p-lab.cz/spojka-hadicova-system-keck?v=R035451_V_7406	15	96
	R034351			10	84
3D printing material	PETG	Prusa Research a. s.	https://www.prusa3d.com/cs/produkt/prusament-petg-jet-black-2kg/	4 kg	95
Rubber hose insulation	KAIFLEX EF	HORNBACH BAUMARKT CS, s r. o.	https://www.hornbach.cz/p/potrubni-izolace-kaiflex-ef-tube-ef-o-22-mm-sirka-vrstvy-13-mm-delka-1-m/5852909/	8	12
Other components	Fittings; hose holders, reducers; bolts and nuts	-	-	-	239
				Total:	3,010

Author contribution

465 Concept – JH, OG; Methodology – JK, JH, OG; Software – JH, OG; Investigation – JK; Validation – JK, KF, VS, MS, LV;
Visualization – JK; Writing – original draft preparation – JK, KF; Writing – review & editing – JK, JH, OG, KF, VS, MS, NO,
LV; Supervision – LV.

Competing interests

One of the co-authors (NO) is a member of the Editorial Board of the journal Hydrology and Earth System Sciences.

470 Acknowledgements

This work was supported by the Czech Academy of Sciences [RVO: 67985874]; the research programme Strategy AV21
Water for Life; Czech Science Foundation [GA CR 22-12837S]; Faculty of Science, Charles University in Prague [SVV 244-
2606941] and German Federal Environmental Foundation [DBU]. The authors warmly thank Petr Filip at the Institute of
Hydrodynamics of the Czech Academy of Sciences for his help in the final revision of the manuscript. We are also grateful to

475 ~~two-three~~ anonymous reviewers for their useful comments on an earlier version of the manuscript.

References

- Araguás-Araguás, L., Rozanski, K., Gonfiantini, R., Louvat, D.: Isotope effects accompanying vacuum extraction of soil water
for stable isotope analyses, *Journal of Hydrology*, 168(1–4), 159–171, doi:10.1016/0022-1694(94)02636-P, 1995
- 480 ~~Ceperley, N., Gimeno, T. E., Jacobs, S. R., Beyer, M., Dubbert, M., Fischer, B., Geris, J., Holke, L., Kübert, A., Le Gall, S.,
Lehmann, M. M., Llorens, P., Millar, C., Penna, D., Prieto, I., Radolinski, J., Scandellari, F., Stockinger, M., Stumpp, C.,
Tetzlaff, D., van Meerveld, I., Werner, C., Yildiz, O., Zucco, G., Barbeta, A., Orłowski, N., Rothfuss, Y.: Toward a
common methodological framework for the sampling, extraction, and isotopic analysis of water in the Critical Zone to
study vegetation water use, *WIREs Water*, 11(4), e1727, doi:10.1002/wat2.1727, 2024~~
- Barrow, N. J., Whelan, B. R.: A study of a method for displacing soil solution by centrifuging with an immiscible liquid,
485 *Journal of Environmental Quality*, 9(2), 315–319, doi:10.2134/jeq1980.00472425000900020031x, 1980
- Batley, G., Giles, M.: Solvent displacement of sediment interstitial waters before trace metal analysis, *Water Research*, 13(9),
879–886, doi:10.1016/0043-1354(79)90223-9, 1979
- Berrie, J. A., Machin, D.: The sorption and diffusion of water in silicone rubbers: Part I. Unfilled rubbers, *Journal of
Macromolecular Science, Part B*, 3(4), 645–672, doi:10.1080/00222346908217112, 1969
- 490 Böttcher, G., Brumsack, H.-J., Heinrichs, H., Pohlmann, M.: A new high-pressure squeezing technique for pore fluid extraction
from terrestrial soils, *Water, Air, and Soil Pollution*, 94(3-4), 289–296, doi:10.1007/BF02406064, 1997

- Brumsack, H., Zuleger, E., Gohn, E., Murray, R.: Stable and radiogenic isotopes in pore waters from leg 127, Japan Sea, In Pisciotta, K., Ingle, J., von Breyman, M., Barron, J.: Proceedings of the Ocean Drilling Program, 127/128 Part 1 Scientific Results, 127/128, 635–650, doi:10.2973/odp.proc.sr.127128-1.165.1992, 1992
- 495 [Ceperley, N., Gimeno, T. E., Jacobs, S. R., Beyer, M., Dubbert, M., Fischer, B., Geris, J., Holko, L., Kübert, A., Le Gall, S., Lehmann, M. M., Llorens, P., Millar, C., Penna, D., Prieto, I., Radolinski, J., Scandellari, F., Stockinger, M., Stumpp, C., Tetzlaff, D., van Meerveld, I., Werner, C., Yildiz, O., Zuecco, G., Barbata, A., Orłowski, N., Rothfuss, Y.: Toward a common methodological framework for the sampling, extraction, and isotopic analysis of water in the Critical Zone to study vegetation water use. *WIREs Water*, 11\(4\), e1727, doi:10.1002/wat2.1727, 2024](#)
- 500 Craig, H.: Standard for reporting concentrations of deuterium and oxygen-18 in natural waters, *Science*, 133(3467), 1833–1834, doi:10.1126/science.133.3467.1833, 1961
- Dansgaard, W.: Stable isotopes in precipitation. *Tellus* 16(4), 436–468, doi:10.1111/j.2153-3490.1964.tb00181.x, 1964
- Dalton, F. N.: Plant root water extraction studies using stable isotopes, *Plant Soil*, 111(2), 217–221, doi:10.1007/BF02139942, 1988
- 505 Gaj, M., Beyer, M., Koeniger, P., Wanke, H., Hamutoko, J., Himmelsbach, T.: In-situ unsaturated zone stable water isotope (^2H and ^{18}O) measurements in semi-arid environments: a soil water balance, *Hydrology and Earth System Sciences*, 20, 715–731, doi:10.5194/hess-20-715-2016, 2016
- Gaj, M., Kaufhold, S., McDonnell, J. J.: Potential limitation of cryogenic vacuum extractions and spiked experiments, *Rapid Communications in Mass Spectrometry*, 31, 821–823, doi:10.1002/rcm.7850, 2017
- 510 Gaj, M., McDonnell, J. J.: Possible soil tension controls on the isotopic equilibrium fractionation factor for evaporation from soil, *Hydrological Processes*, 33(11), 1629–1634, doi:10.1002/hyp.13418, 2019
- Garvelmann, J., Kuells, C., Weiler, M.: A porewater-based stable isotope approach for the investigation of subsurface hydrological processes, *Hydrology and Earth System Sciences*, 16(2), 631–640, doi:10.5194/hess-16-631-2012, 2012
- Goebel, T. S., Lascano, R. J.: System for high throughput water extraction from soil material for stable isotope analysis of
- 515 water, *Journal of Analytical Sciences, Methods and Instrumentation*, 02(04), 203–207, doi:10.4236/jasmi.2012.24031, 2012
- Gralher, B., Herbstritt, B., Weiler, M., Wassenaar, L. I., Stumpp, C.: Correcting Laser-Based Stable Isotope Reading Biased by Carrier Gas Changes, *Environmental Science & Technology*, 50(13), 7047–7081, doi:10.1021/acs.est.6b01124, 2016
- Hendry, M. J., Schmeling, E., Wassenaar, L. I., Barbour, S. L., Pratt, D.: Determining the stable isotope composition of pore
- 520 water from saturated and unsaturated zone core: improvements to the direct vapour equilibration laser spectrometry method, *Hydrology and Earth System Sciences*, 19(11), 4427–4440, doi:10.5194/hess-19-4427-2015, 2015
- Hsieh, J. C. C., Savin, S. M., Kelly, E. F., Chadwick, O. A.: Measurement of soil-water $\delta^{18}\text{O}$ values by direct equilibration with CO_2 , *Geoderma*, 82(1-3), 255–268, doi:10.1016/S0016-7061(97)00104-3, 1998
- Ignatev, A., Velivetchkaia, T., Sugimoto, A., Ueta, A.: A soil water distillation technique using He-purging for stable isotope
- 525 analysis, *Journal of Hydrology*, 498, 265–273, doi:10.1016/j.jhydrol.2013.06.032, 2013

- Ishimaru, H., Itoh, K., Ishigaki, T., Furutate, M.: Fast pump-down aluminum ultrahigh vacuum system, *Journal of Vacuum Science & Technology*, 10, 547–552, doi:10.1116/1.578186, 1992
- Jusserand, C.: Pore water extraction from sediment and soil: Oxygen-18 abundances comparisons between different techniques. First results, *Catena*, 7(1), 87–96, doi:10.1016/S0341-8162(80)80006-3, 1980
- 530 Kelln, C. J., Wassenaar, L. I., Hendry, M. J.: Stable Isotopes ($\delta^{18}\text{O}$, $\delta^2\text{H}$) of Pore Waters in Clay-Rich Aquitards: A Comparison and Evaluation of Measurement Techniques, *Ground Water Monitoring & Remediation*, 21(2), 108–116, doi:10.1111/j.1745-6592.2001.tb00306.x, 2001
- Kendall, C., Coplen, T. B.: Multi-sample conversion of water to hydrogen by zinc for stable isotope determination, *Analytical Chemistry*, 57(7), 1437–1440, doi:10.1021/ac00284a058, 1985
- 535 Koehler, G., Wassenaar, L. I., Hendry, M. J.: An Automated Technique for Measuring δD and $\delta^{18}\text{O}$ Values of Porewater by Direct CO_2 and H_2 Equilibration, *Analytical Chemistry*, 72(22), 5659–5664, doi:10.1021/ac000498n, 2000
- Koeniger, P., Marshall, J. D., Link, T., Mulch, A.: An inexpensive, fast, and reliable method for vacuum extraction of soil and plant water for stable isotope analyses by mass spectrometry, *Rapid Communication in Mass Spectrometry*, 25(20), 3041–3048, doi:10.1002/rcm.5198, 2011
- 540 Kübert, A., Paulus, S., Dahlmann, A., Werner, C., Rothfuss, Y., Orłowski, N., Dubbert, M.: Water stable isotopes in ecohydrological field research: comparison between in situ and destructive monitoring methods to determine soil water isotopic signatures, *Plant Science*, 11, doi:10.3389/fpls.2020.00387, 2020
- Leaney, F. W., Smettem, K. R. J., Chittleborough, D. J.: Estimating the contribution of preferential flow to subsurface runoff from a hillslope using deuterium and chloride, *Journal of Hydrology*, 147, 83–103, doi:10.1016/0022-1694(93)90076-L,
- 545 1993
- McConville, C., Kalin, R. M., Flood, D.: Direct equilibration of soil water for $\delta^{18}\text{O}$ analysis and its application to tracer studies, *Rapid Communication in Mass Spectrometry*, 13(13), 1339–1345, doi:10.1002/(SICI)1097-0231(19990715)13:13<1339::AID-RCM559>3.0.CO;2-N, 1999
- Meißner, M., Köhler, M., Schwendenmann, L., Hölscher, D., Dyckmans, J.: Soil water uptake by trees using water stable isotopes ($\delta^2\text{H}$ and $\delta^{18}\text{O}$) – a method test regarding soil moisture, texture and carbonate, *Plant Soil*, 376(1-2), 327–335, doi:10.1007/s11104-013-1970-z, 2014
- 550 Mora, G., Jahren, A. H.: Isotopic evidence for the role of plant development on transpiration in deciduous forests of southern United States, *Global Biogeochemical Cycles*, 17(2), 13–1–13–7. doi:10.1029/2002GB001981, 2003
- Mubarak, A., Olsen, R.: Immiscible displacement of soil solution by centrifugation, *Soil Science Society of America Journal*,
- 555 40(2), 329–331, ISSN/ISBN: 0361-5995, 1976
- Munksgaard, N. C., Cheesman, A. W., Wurster, C. M., Cernusak, L. A., Bird, M. I.: Microwave extraction–isotope ratio infrared spectroscopy (ME-IRIS): a novel technique for rapid extraction and in-line analysis of $\delta^{18}\text{O}$ and $\delta^2\text{H}$ values of water in plants, soils and insects, *Rapid Communication in Mass Spectrometry*, 28(20), 2151–2161, doi:10.1002/rcm.7005, 2014

- 560 Newberry, S. L., Prechsl, U. E., Pace, M., Kahmen, A.: Tightly bound soil water introduces isotopic memory effects on mobile and extractable soil water pools, *Isotopes in Environmental and Health Studies*, 52(4), 368–381, doi:10.1080/10256016.2017.1302446, 2017
- O’Kelly, B. C.: Accurate Determination of Moisture Content of Organic Soils Using the Oven Drying Method, *Drying Technology*, 22(7), 1767–1776, doi:10.1081/DRT-200025642, 2004
- 565 O’Kelly, B. C.: Oven-Drying Characteristics of Soil of Different Origins, *Drying Technology*, 23(5), 1141–1149, doi:10.1081/DRT-200059149, 2005
- Orlowski, N., Frede, H.-G., Brüggemann, N., Breuer, L.: Validation and application of a cryogenic vacuum extraction system for soil and plant water extraction for isotope analysis, *Journal of Sensors and Sensor Systems*, 2(2), 179–193, doi:10.5194/jsss-2-179-2013, 2013
- 570 Orlowski, N., Breuer, L., McDonnell, J. J.: Critical issues with cryogenic extraction of soil water for stable isotope analysis, *Ecohydrology*, 9, 3–10, doi:10.1002/eco.1722, 2016a
- Orlowski, N., Pratt, D. L., McDonnell, J. J.: Intercomparison of soil pore water extraction methods for stable isotope analysis, *Hydrological Processes*, 30, 3433–3449, doi:10.1002/hyp.10870, 2016b
- Orlowski, N., Breuer, L., Angeli, N., Boeckx, P., Brumbt, C., Cook, C. S., Dubbert, M., Dyckmans, J., Gallagher, B., Gralher, B., Herbstritt, B., Hervé-Fernández, P., Hissler, C., Koeniger, P., Legout, A., Macdonald, C. J., Oyarzún, C., Redelstein, R., Seidler, C., Siegwolf, R., Stumpp, C., Thomsen, S., Weiler, M., Werner, C., McDonnell, J. J.: Inter-laboratory comparison of cryogenic water extraction systems for stable isotope analysis of soil water, *Hydrology and Earth System Sciences*, 22(7), 3619–3637, doi:10.5194/hess-22-3619-2018, 2018
- 575 Orlowski, N., Pratt, D. L., McDonnell, J. J.: Intercomparison of soil pore water extraction methods for stable isotope analysis and interpretation of hillslope runoff sources, *Hydrological Processes*, 33(22), 2939–2954, doi:10.1002/hyp.13539, 2019
- Orlowski, N., Breuer, L.: Sampling soil water along pF curve for $\delta^2\text{H}$ and $\delta^{18}\text{O}$ analysis, *Hydrological Processes*, 34(25), 4959–4972, doi:10.1002/hyp.13916, 2020
- Penna, D., Stenni, B., Šanda, M., Wrede, S., Bogaard, T. A., Gobbi, A., Borga, M., Fischer, B. M. C., Bonazza, M., Chárová, Z.: On the reproducibility and repeatability of laser absorption spectroscopy measurements for $\delta^2\text{H}$ and $\delta^{18}\text{O}$ isotopic analysis, *Hydrology and Earth System Sciences*, 14, 1551–1566, doi:10.5194/hess-14-1551-2010, 2010
- 585 Penna, D., Stenni, B., Šanda, M., Wrede, S., Bogaard, T. A., Micheline, M., Fischer, B. M. C., Gobbi, A., Mantese, N., Zuecco, G., Borga, M., Bonazza, M., Sobotková, M., Čejková, B., Wassenaar, L. I.: Technical Note: Evaluation of between-sample memory effects in the analysis of $\delta^2\text{H}$ and $\delta^{18}\text{O}$ of water samples measured by laser spectrometers, *Hydrology and Earth System Sciences*, 16, 3925–3933, doi:10.5194/hess-16-3925-2012, 2012
- 590 Peters, L. I., Yakir, D.: A direct and rapid leaf water extraction method for isotopic analysis, *Rapid Communication in Mass Spectrometry*, 22(18), 2929–2936, doi:10.1002/rcm.3692, 2008
- Revesz, K., Woods, P. H.: A method to extract soil water for stable isotope analysis, *Journal of Hydrology*, 115(1-4), 397–406, doi:10.1016/0022-1694(90)90217-L, 1990

- Rothfuss, Y., Vereecken, H., Brüggemann, N.: Monitoring water stable isotopic composition in soils using gas-permeable tubing and infrared laser absorption spectroscopy, *Water Resources Research*, 49, 1–9, doi:10.1002/wrcr.20311, 2013
- 595 Rothfuss, Y., Merz, S., Vanderborght, J., Hermes, N., Weuthen, A., Pohlmeier, A., Vereecken, H., Brüggemann, N.: Long-term and high-frequency non-destructive monitoring of water stable isotope profiles in an evaporating soil column, *Hydrology and Earth System Sciences*, 19(10), 4067–4080, doi:10.5194/hess-19-4067-2015, 2015
- Scrimgeour, C. M.: Measurement of plant and soil water isotope composition by direct equilibration methods, *Journal of Hydrology*, 172(1-4), 261–274, doi:10.1016/0022-1694(95)02716-3, 1995
- 600 Sprenger, M., Herbstritt, B., Weiler, M.: Established methods and new opportunities for pore water stable isotope analysis, *Hydrological Processes*, 29(25), 5174–5192, doi:10.1002/hyp.10643, 2015
- Stumpp, C., Brüggemann, N., Wingate, L.: Stable Isotope Approaches in Vadose Zone Research, *Vadose Zone Journal*, 17(1), 1–7, doi:10.2136/vzj2018.05.0096, 2018
- 605 Thorburn, P. J., Walker, G. R., Brunel, J.-P.: Extraction of water from Eucalyptus trees for analysis of deuterium and oxygen-18: laboratory and field techniques, *Plant, Cell & Environment*, 16(3), 269–277, doi:10.1111/j.1365-3040.1993.tb00869.x, 1993
- Volkman, T. H. M., Weiler, M.: Continual in situ monitoring of pore water stable isotopes in the subsurface, *Hydrology and Earth System Sciences*, 18(5), 1819–1833, doi:10.5194/hess-18-1819-2014, 2014
- 610 Walker, G. R., Woods, P. H., Allison, G. B.: Interlaboratory comparison of methods to determine the stable isotope composition of soil water, *Chemical Geology*, 111(1-4), 297–306, doi:10.1016/0009-2541(94)90096-5, 1994
- Wassenaar, L. I., Hendry, M. J., Chostner, V. L., Lis, G. P.: High Resolution Pore Water $\delta^2\text{H}$ and $\delta^{18}\text{O}$ Measurements by $\text{H}_2\text{O}_{(\text{liquid})}$ - $\text{H}_2\text{O}_{(\text{vapor})}$ Equilibration Laser Spectroscopy, *Environmental Science & Technology*, 42(24), 9262–9267, doi:10.1021/es802065s, 2008
- 615 Wassenaar, L. I., Ahmad, M., Aggarwal, P., van Duren, M., Pöltenstein, L., Araguas, L., Kurttas, T.: Worldwide proficiency test for routine analysis of $\delta^2\text{H}$ and $\delta^{18}\text{O}$ in water by isotope-ratio mass spectrometry and laser absorption spectroscopy, *Rapid Communication in Mass Spectrometry*, 26, 1641–1648, doi:10.1002/rcm.6270, 2012
- Wershaw, R. L., Friedman, I., Heller, S. J., Frank, P. A.: Hydrogen isotopic fractionation of water passing through trees, In *Advances in Organic Geochemistry: Proceedings of the Third International Congress*, edited by F. Hobson and M. Speers, 620 55–67, Pergamon Press Ltd., Elsevier, New York, USA, 1966
- West, A. G., Patrickson, S. J., Ehleringer, J. R.: Water extraction times for plant and soil materials used in stable isotope analysis, *Rapid Communication in Mass Spectrometry*, 20(8), 1317–1321, doi:10.1002/rcm.2456, 2006
- White, J. W. C., Cook, E. R., Lawrence, J. R., Wallace S., B.: The D/H ratios of sap in trees: Implications for water sources and tree ring D/H ratios. *Geochimica et Cosmochimica Acta*, 49(1), 237–246, doi:10.1016/0016-7037(85)90207-8, 1985
- 625 Yang, B., Dossa, G. G. O., Hu, Y. H., Liu, L. L., Meng, X. J., Du, Y. Y., Li, J. Y., Zhu, X. A., Zhang, Y. J., Singh, A. K., Yuan, X., Wu, J. E., Zakari, S., Liu, W. J., Song, L.: Uncorrected soil water isotopes through cryogenic vacuum distillation

may lead to a false estimation on plant water source, *Methods in Ecology and Evolution*, 6, 1443–1456, doi:10.1111/2041-210X.14107, 2023

630 Zhu, Q.-Z., Sun, Q., Su, Z.-G., Xie, M.-M., Song, J.-Y., Shan, Y.-B., Wang, N., Chu, G.- Q.: A Soil Water Extraction Method with Accelerated Solvent Extraction Technique for Stable Isotope Analysis, *Chinese Journal of Analytical Chemistry*, 42(9), 1270–1275, doi:10.1016/S1872-2040(14)60766-0, 2014